

High-Volume TSP Sampler
5-Point Calibration Record

Location : AM1(ICC)
 Calibrated by : K.T.Ho
 Date : 08/07/2024

Sampler

Model : TE-5170
 Serial Number : S/N 0767

Calibration Orifice and Standard Calibration Relationship

Serial Number : 2454
 Next Calibration Date : 15 December 2024
 Slope (m) : 2.07544
 Intercept (b) : -0.03205
 Correlation Coefficient(r) : 0.99999

Standard Condition

Pstd (hpa) : 1013
 Tstd (K) : 298.18

Calibration Condition


Pa (hpa) : 1008
 Ta(K) : 305

| Resistance Plate | dH [green liquid] (inch water) | Z | X=Qstd (cubic meter/min) | IC (chart) | Y (corrected) |
|------------------|-----------------------------------|-------|-----------------------------|---------------|------------------|
| 1 18 holes | 12.2 | 3.444 | 1.675 | 62 | 61.14 |
| 2 13 holes | 8.8 | 2.925 | 1.425 | 52 | 51.28 |
| 3 10 holes | 6.4 | 2.495 | 1.217 | 40 | 39.45 |
| 4 7 holes | 4.0 | 1.972 | 0.966 | 30 | 29.58 |
| 5 5 holes | 2.6 | 1.590 | 0.782 | 18 | 17.75 |

Notes: $Z = \sqrt{dH(Pa/Pstd)(Tstd/Ta)}$, $X = Z/m - b$, $Y(\text{Corrected Flow}) = IC * \sqrt{Pa/Pstd)(Tstd/Ta)}$

Sampler Calibration Relationship

Slope(m): 48.113 Intercept(b): -18.519 Correlation Coefficient(r): 0.9969

Checked by: 

 Magnum Fan

Date: 10/07/2024

High-Volume TSP Sampler
5-Point Calibration Record

Location : AM1(ICC)
 Calibrated by : K.T.Ho
 Date : 06/09/2024

Sampler

Model : TE-5170
 Serial Number : S/N 0767

Calibration Orifice and Standard Calibration Relationship

Serial Number : 2454
 Next Calibration Date : 15 December 2024
 Slope (m) : 2.07544
 Intercept (b) : -0.03205
 Correlation Coefficient(r) : 0.99999

Standard Condition

Pstd (hpa) : 1013
 Tstd (K) : 298.18

Calibration Condition


Pa (hpa) : 1009
 Ta(K) : 302

| Resistance Plate | dH [green liquid] (inch water) | Z | X=Qstd (cubic meter/min) | IC (chart) | Y (corrected) |
|------------------|-----------------------------------|-------|-----------------------------|---------------|------------------|
| 1 18 holes | 10.2 | 3.167 | 1.541 | 60 | 59.49 |
| 2 13 holes | 7.6 | 2.733 | 1.332 | 50 | 49.58 |
| 3 10 holes | 6.0 | 2.429 | 1.186 | 40 | 39.66 |
| 4 7 holes | 4.0 | 1.983 | 0.971 | 28 | 27.76 |
| 5 5 holes | 2.6 | 1.599 | 0.786 | 18 | 17.85 |

Notes: $Z = \sqrt{dH(Pa/Pstd)(Tstd/Ta)}$, $X = Z/m - b$, $Y(\text{Corrected Flow}) = IC * \sqrt{Pa/Pstd}(Tstd/Ta)$

Sampler Calibration Relationship

Slope(m): 56.036 Intercept(b): -26.314 Correlation Coefficient(r): 0.9990

Checked by: 

 Magnum Fan

Date: 09/09/2024



Certificate of Calibration

| Calibration Certification Information | | | |
|---------------------------------------|-----------------------------|-----------|-------|
| Cal. Date: December 15, 2023 | Rootsmeter S/N: 438320 | Ta: 295 | °K |
| Operator: Jim Tisch | | Pa: 748.5 | mm Hg |
| Calibration Model #: TE-5025A | Calibrator S/N: 2454 | | |

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4250 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0090 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9040 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8610 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7110 | 12.8 | 8.00 |

| Data Tabulation | | | | | |
|-----------------|---------------|--|-----------|-------------|------------------------------------|
| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H (Ta/Pa)}$ (y-axis) |
| 0.9907 | 0.6952 | 1.4106 | 0.9957 | 0.6988 | 0.8878 |
| 0.9864 | 0.9776 | 1.9949 | 0.9914 | 0.9826 | 1.2556 |
| 0.9844 | 1.0890 | 2.2304 | 0.9894 | 1.0945 | 1.4037 |
| 0.9832 | 1.1420 | 2.3393 | 0.9882 | 1.1478 | 1.4723 |
| 0.9779 | 1.3754 | 2.8213 | 0.9829 | 1.3824 | 1.7756 |
| QSTD | m= | 2.07544 | QA | m= | 1.29961 |
| | b= | -0.03205 | | b= | -0.02017 |
| | r= | 0.99999 | | r= | 0.99999 |

| Calculations | |
|---|---|
| Vstd= $\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$ | Va= $\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$ |
| Qstd= $Vstd / \Delta Time$ | Qa= $Va / \Delta Time$ |
| For subsequent flow rate calculations: | |
| Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= $1/m \left(\left(\sqrt{\Delta H (Ta/Pa)} \right) - b \right)$ |

| Standard Conditions | |
|---|-----------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: calibrator manometer reading (in H2O) | |
| ΔP: rootsmeter manometer reading (mm Hg) | |
| Ta: actual absolute temperature (°K) | |
| Pa: actual barometric pressure (mm Hg) | |
| b: intercept | |
| m: slope | |

| RECALIBRATION |
|--|
| US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30 |



SUB-CONTRACTING REPORT

| | | | |
|---------|--|----------------|---------------|
| CONTACT | : MR MAGNUM FAN | WORK ORDER | : HK2404331 |
| CLIENT | : ENVIROTECH SERVICES CO. | | |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD, TUEN MUN, N.T. HK | SUB-BATCH | : 1 |
| | | DATE RECEIVED | : 19-JAN-2024 |
| | | DATE OF ISSUE | : 31-JAN-2024 |
| PROJECT | : --- | NO. OF SAMPLES | : 1 |
| | | CLIENT ORDER | : --- |

General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
 - Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
 - Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
 - Calibration was subcontracted to Envirotech Services Company.
-

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

11/F Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong
Tel. +852 2610 1044 Fax +852 2610 2021 www.alsglobal.com

WORK ORDER : HK2404331
SUB-BATCH : 1
CLIENT : ENVIROTECH SERVICES CO
PROJECT : ----



| ALS Lab ID | Client's Sample ID | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2404331-001 | Sibata LD-5R (831656) | Equipments | 19-Jan-2024 | S/N: 831656 |



Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust Monitor
Manufacturer: Sibata LD-5R
Serial No.: 831656
Equipment Ref.: N/A
ALS Job Order: HK2402531

Standard Equipment

Standard Equipment: High Volume Sampler (TSP)
Location: Envirotech Room (Calibration Room)
Equipment Ref.: HVS 8162
Last Calibration Date: 12-Jan-2024


Equipment Verification Results:

Verification Date: 13-Jan-2024

| Hour | Time | Mean Temp °C | Mean Pressure (hpa) | Concentration in µg/m³ (Standard Equipment) (Y-Axis) | Concentration in µg/m³ (Calibrated Equipment) (X-Axis) |
|------------|-----------|--------------|---------------------|--|--|
| 1hr 00mins | 0900-1000 | 19.5 | 1018 | 43 | 31 |
| 2hr 00mins | 1005-1205 | 23.5 | 1022 | 161 | 121 |
| 3hr 00mins | 1330-1630 | 24.0 | 1022 | 184 | 145 |

Linear Regression of Y or X

Slope (K-factor): 1.2820(µg/m³)/CPM
Correlation Coefficient (R): 0.9993
Date of Issue: 19-Jan-2024

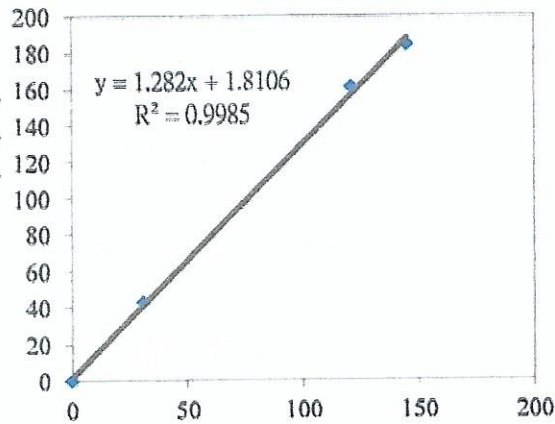

Remarks:

- 1. Strong Correlation (>0.8)
- 2. Factor 1.2820 (µg/m³)/CPM should be applied for TSP monitoring

*If R<0.5, repair or verification is required for the equipment

Operator: P.F.Yeung Signature *Fai* Date: 19 January 2024

QC Reviewer: K.F.Ho Signature *fat* Date: 19 January 2024

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

| | | |
|--|------------------------|-----------|
| Location : Rm. 712, My Loft, Tuen Mun | Date of Calibration: | 12-Jan-24 |
| HVS ID: 8162 | Next Calibration Date: | 12-Mar-24 |
| Name and Model : TISCH HVS Model TE-5170 | Operator: | P.F.Yeung |

CONDITIONS

| | | | |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1018 | Corrected Pressure (mm Hg) | 763.7 |
| Temperature (°C) | 20.0 | Temperature (K) | 293 |

CALIBRATION ORIFICE

| | | | |
|----------|----------|----------------|----------|
| Make: | TISCH | Qstd Slope | 2.07544 |
| Model: | TE-5025A | Qstd Intercept | -0.03205 |
| Serial#: | 2454 | | |

CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|--|
| 18 | 6.6 | 6.6 | 13.2 | 1.786 | 61 | 61.68 | Slope= 34.506 Intercept= -0.179 Corr. Coeff.= 0.9986 |
| 13 | 5.3 | 5.3 | 10.6 | 1.602 | 54 | 54.61 | |
| 10 | 4.5 | 4.5 | 9.0 | 1.477 | 50 | 50.56 | |
| 7 | 2.7 | 2.7 | 5.4 | 1.148 | 40 | 40.45 | |
| 5 | 1.7 | 1.6 | 3.3 | 0.901 | 30 | 30.34 | |

Calculations:

$$Qstd = 1/m[\text{sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m(I[\text{sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

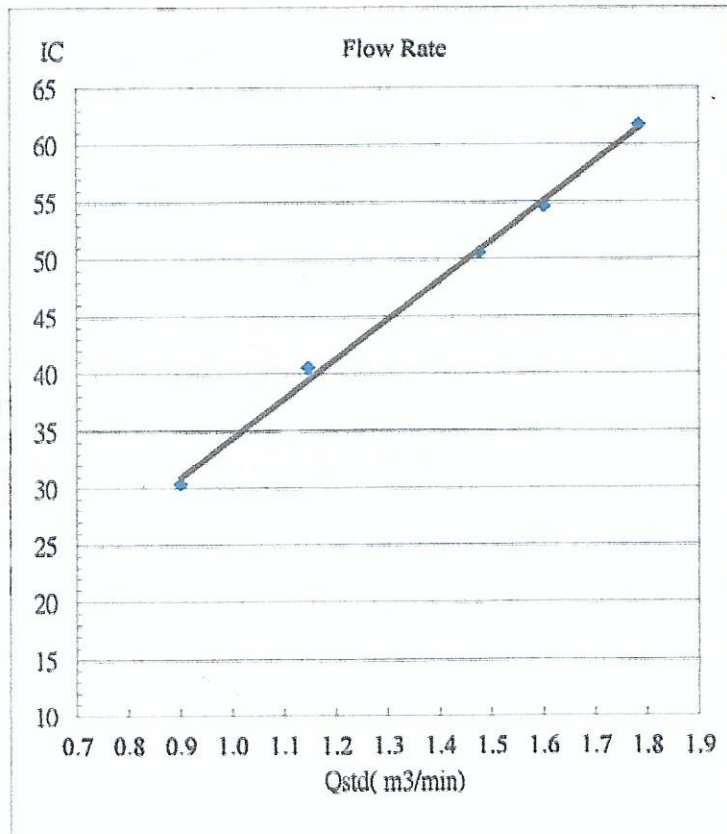

Certificate of Calibration

| Calibration Certification Information | | | |
|---------------------------------------|-----------------------------|-----------|-------|
| Cal. Date: December 15, 2023 | Rootsmeter S/N: 438320 | Ta: 295 | °K |
| Operator: Jim Tisch | | Pa: 748.5 | mm Hg |
| Calibration Model #: TE-5025A | Calibrator S/N: 2454 | | |

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4250 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0090 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9040 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8610 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7110 | 12.8 | 8.00 |

| Data Tabulation | | | | | |
|-----------------|---------------|--|-----------|-------------|---|
| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(Ta/Pa \right)}$ (y-axis) |
| 0.9907 | 0.6952 | 1.4106 | 0.9957 | 0.6988 | 0.8878 |
| 0.9864 | 0.9776 | 1.9949 | 0.9914 | 0.9826 | 1.2556 |
| 0.9844 | 1.0890 | 2.2304 | 0.9894 | 1.0945 | 1.4037 |
| 0.9832 | 1.1420 | 2.3393 | 0.9882 | 1.1478 | 1.4723 |
| 0.9779 | 1.3754 | 2.8213 | 0.9829 | 1.3824 | 1.7756 |
| QSTD | m= | 2.07544 | QA | m= | 1.29961 |
| | b= | -0.03205 | | b= | -0.02017 |
| | r= | 0.99999 | | r= | 0.99999 |

| Calculations | |
|---|--|
| Vstd= $\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$ | Va= $\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$ |
| Qstd= Vstd/ΔTime | Qa= Va/ΔTime |
| For subsequent flow rate calculations: | |
| Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= $1/m \left(\left(\sqrt{\Delta H \left(Ta/Pa \right)} \right) - b \right)$ |

| Standard Conditions | |
|---|-----------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: calibrator manometer reading (in H2O) | |
| ΔP: rootsmeter manometer reading (mm Hg) | |
| Ta: actual absolute temperature (°K) | |
| Pa: actual barometric pressure (mm Hg) | |
| b: intercept | |
| m: slope | |

| RECALIBRATION |
|--|
| US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30 |



SUB-CONTRACTING REPORT

| | | | |
|---------|--|----------------|---------------|
| CONTACT | : MR MAGNUM FAN | WORK ORDER | : HK2351432 |
| CLIENT | : ENVIROTECH SERVICES CO. | | |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD, TUEN MUN, N.T. HK | SUB-BATCH | : 1 |
| | | DATE RECEIVED | : 18-DEC-2023 |
| | | DATE OF ISSUE | : 27-DEC-2023 |
| PROJECT | : ---- | NO. OF SAMPLES | : 1 |
| | | CLIENT ORDER | : ---- |

General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
- Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
- Calibration was subcontracted to Envirotech Services Company.
- Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong
Tel. +852 2610 1044 Fax +852 2610 2021 www.alsglobal.com

WORK ORDER : HK2351432
SUB-BATCH : 1
CLIENT : ENVIROTECH SERVICES CO.
PROJECT : ----



| ALS Lab ID | Client's Sample ID | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2351432-001 | Sibata LD-3B (235780) | Equipments | 09-Dec-2023 | S/N: 235780 |



Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust Monitor
Manufacturer: Sibata LD-3B
Serial No.: 235780
Equipment Ref.: N/A
ALS Job Order: HK2349963

Standard Equipment

Standard Equipment: High Volume Sampler (TSP)
Location: Envirotech Room (Calibration Room)
Equipment Ref.: HVS 8162
Last Calibration Date: 13-Oct-2023


Equipment Verification Results:

Verification Date: 9-Dec-2023

| Hour | Time | Mean Temp °C | Mean Pressure (hpa) | Concentration in µg/m³ (Standard Equipment) Y(axis) | Concentration in µg/m³ (Calibrated Equipment) x(axis) |
|------------|-----------|--------------|---------------------|--|--|
| 1hr 00mins | 1010-1110 | 26.5 | 1016.0 | 112 | 88 |
| 2hr 00mins | 1300-1500 | 26.2 | 1015.5 | 165 | 135 |
| 3hr 00mins | 1505-1805 | 26.2 | 1015.5 | 300 | 215 |

Linear Regression of Y or X

Slope (K-factor): 1.3803(µg/m³)/CPM
Correlation Coefficient (R): 0.9960
Date of Issue: 15-Dec-2023

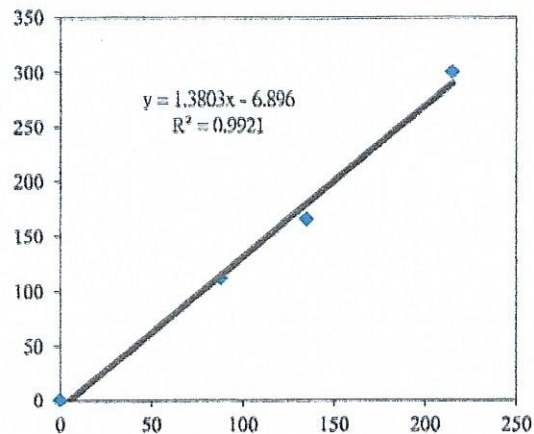

Remarks:

- 1. Strong Correlation (>0.8)
- 2. Factor 1.3803 (µg/m³)/CPM should be applied for TSP monitoring

*If R<0.5, repair or verification is required for the equipment

Operator: P.F.Yeung Signature *PfY* Date: 15 December 2023

QC Reviewer: K.F.Ho Signature *KfH* Date: 15 December 2023

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

| | | |
|--|------------------------|-----------|
| Location : Rm. 712, My Loft, Tuen Mun | Date of Calibration: | 13-Oct-23 |
| HVS ID: 8162 | Next Calibration Date: | 12-Dec-23 |
| Name and Model : TISCH HVS Model TE-5170 | Operator: | P.F.Yeung |

CONDITIONS

| | | | |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1015 | Corrected Pressure (mm Hg) | 762.1 |
| Temperature (°C) | 28.9 | Temperature (K) | 293 |

CALIBRATION ORIFICE

| | | | |
|----------|----------|----------------|----------|
| Make: | TISCH | Qstd Slope | 2.06918 |
| Model: | TE-5025A | Qstd Intercept | -0.04220 |
| Serial#: | 2454 | | |

CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|---|
| 18 | 6.5 | 6.5 | 13.0 | 1.806 | 62 | 63.54 | Slope= 32.843 Intercept= 5.518 Corr. Coeff.= 0.9939 |
| 13 | 4.7 | 4.7 | 9.4 | 1.539 | 56 | 57.39 | |
| 10 | 3.4 | 3.4 | 6.8 | 1.312 | 49 | 50.22 | |
| 7 | 2.3 | 2.2 | 4.5 | 1.071 | 40 | 40.99 | |
| 5 | 1.6 | 1.5 | 3.1 | 0.892 | 33 | 33.82 | |

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

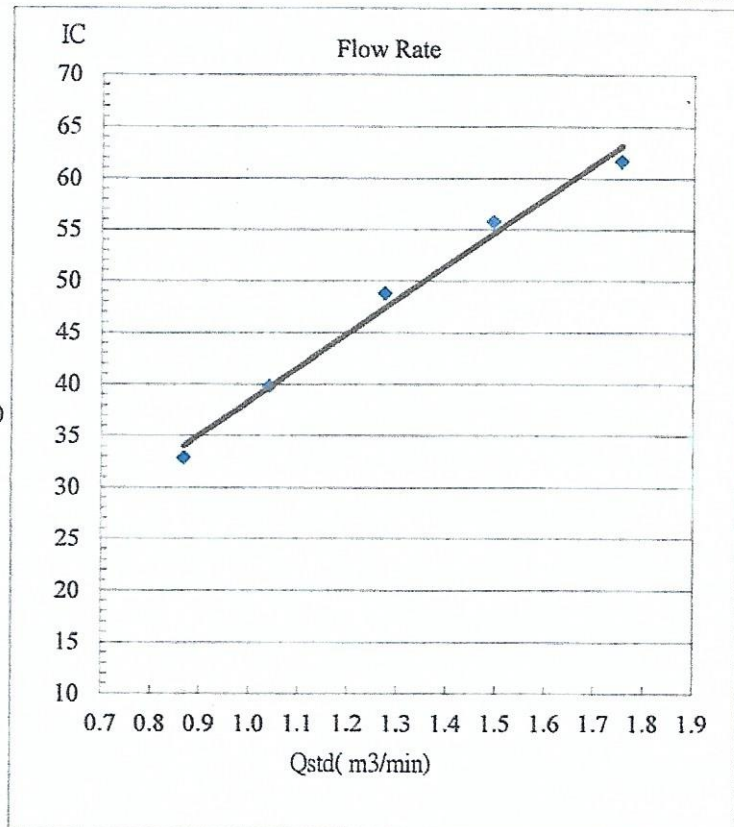

Certificate of Calibration

| Calibration Certification Information | | | |
|---------------------------------------|-----------------------------|-----------|-------|
| Cal. Date: December 15, 2022 | Rootsometer S/N: 438320 | Ta: 295 | °K |
| Operator: Jim Tisch | | Pa: 748.0 | mm Hg |
| Calibration Model #: TE-5025A | Calibrator S/N: 4064 | | |

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4430 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0210 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9170 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8730 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7210 | 12.8 | 8.00 |

| Data Tabulation | | | | | |
|-----------------|---------------|--|-----------|-------------|---|
| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis) |
| 0.9900 | 0.6861 | 1.4101 | 0.9957 | 0.6900 | 0.8881 |
| 0.9858 | 0.9655 | 1.9943 | 0.9914 | 0.9711 | 1.2560 |
| 0.9838 | 1.0728 | 2.2296 | 0.9894 | 1.0790 | 1.4042 |
| 0.9826 | 1.1255 | 2.3385 | 0.9882 | 1.1320 | 1.4728 |
| 0.9772 | 1.3554 | 2.8203 | 0.9829 | 1.3632 | 1.7762 |
| QSTD | m= | 2.10977 | QA | m= | 1.32110 |
| | b= | -0.03782 | | b= | -0.02382 |
| | r= | 0.99998 | | r= | 0.99998 |

| Calculations | | | |
|--|---|-----|--|
| Vstd= | $\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$ | Va= | $\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$ |
| Qstd= | Vstd/ΔTime | Qa= | Va/ΔTime |
| For subsequent flow rate calculations: | | | |
| Qstd= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$ |

| Standard Conditions | |
|---|-----------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: calibrator manometer reading (in H2O) | |
| ΔP: rootsmeter manometer reading (mm Hg) | |
| Ta: actual absolute temperature (°K) | |
| Pa: actual barometric pressure (mm Hg) | |
| b: intercept | |
| m: slope | |

| RECALIBRATION |
|--|
| US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30 |



SUB-CONTRACTING REPORT

| | | | |
|---------|--|----------------|---------------|
| CONTACT | : MR MAGNUM FAN | WORK ORDER | : HK2419604 |
| CLIENT | : ENVIROTECH SERVICES CO. | | |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD, TUEN MUN, N.T. HK | SUB-BATCH | : 1 |
| | | DATE RECEIVED | : 20-MAY-2024 |
| | | DATE OF ISSUE | : 24-MAY-2024 |
| PROJECT | : ---- | NO. OF SAMPLES | : 1 |
| | | CLIENT ORDER | : ---- |

General Comments

- Sample Information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
 - Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
 - Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
 - Calibration was subcontracted to Envirotech Services Company.
-

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong
Tel. +852 2610 1044 Fax +852 2610 2021 www.alsglobal.com

WORK ORDER : HK2419604
SUB-BATCH : 1
CLIENT : ENVIROTECH SERVICES CO.
PROJECT : ----



| ALS Lab ID | Client's Sample ID | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2419604-001 | Sibata LD-3B (235786) | Equipments | 11-May-2024 | S/N: 235786 |

----- END OF REPORT -----



Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust Monitor
Manufacturer: Sibata LD-3B
Serial No.: 235786
Equipment Ref.: N/A
ALS Job Order: HK2418944

Standard Equipment

Standard Equipment: High Volume Sampler (TSP)
Location: Envirotech Room (Calibration Room)
Equipment Ref.: HVS 8162
Last Calibration Date: 25-Mar-2024


Equipment Verification Results:

Verification Date: 11-May-2024

| Hour | Time | Mean Temp °C | Mean Pressure (hpa) | Concentration in µg/m³ (Standard Equipment) (Y-Axis) | Concentration in µg/m³ (Calibrated Equipment) (X-Axis) |
|------------|-----------|--------------|---------------------|--|--|
| 1hr 00mins | 0830-0930 | 26.8 | 1015 | 34 | 28 |
| 2hr 00mins | 0935-1135 | 28.5 | 1015 | 53 | 48 |
| 3hr 00mins | 1310-1610 | 29.5 | 1016 | 133 | 105 |

Linear Regression of Y or X

Slope (K-factor): 1.2673(µg/m³)/CPM
Correlation Coefficient (R): 0.9978
Date of Issue: 19-May-2024

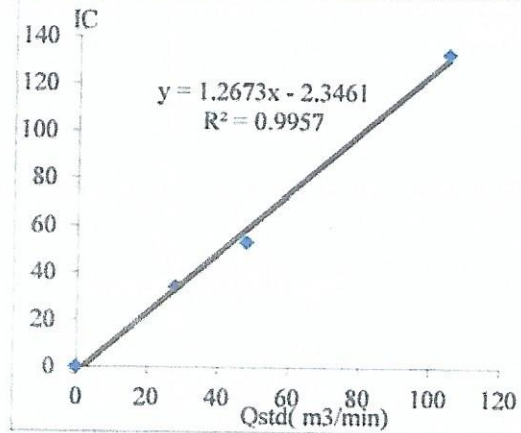

Remarks:

- 1. Strong Correlation (>0.8)
- 2. Factor 1.2673(µg/m³)/CPM should be applied for TSP monitoring

*If R<0.5, repair or verification is required for the equipment

Operator: P.F.Yeung Signature Tai Date: 19 May 2024

QC Reviewer: K.F.Ho Signature Ho Date: 19 May 2024

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

| | |
|--|----------------------------------|
| Location : Rm. 712, My Loft, Tuen Mun | Date of Calibration: 25-Mar-24 |
| HVS ID: 8162 | Next Calibration Date: 24-May-24 |
| Name and Model : TISCH HVS Model TE-5170 | Operator: P.F. Yeung |

CONDITIONS

| | | | |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1016 | Corrected Pressure (mm Hg) | 762.1 |
| Temperature (°C) | 24.5 | Temperature (K) | 297.5 |

CALIBRATION ORIFICE

| | | | |
|----------|----------|----------------|----------|
| Make: | TISCH | Qstd Slope | 2.07544 |
| Model: | TE-5025A | Qstd Intercept | -0.03205 |
| Serial#: | 2454 | | |

CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION Slope= 30.471 Intercept= 5.514 Corr. Coeff.= 0.9994 |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|--|
| 18 | 6.7 | 6.8 | 13.5 | 1.790 | 60 | 60.15 | |
| 13 | 5.5 | 5.6 | 11.1 | 1.625 | 55 | 55.13 | |
| 10 | 4.3 | 4.5 | 8.8 | 1.448 | 49 | 49.12 | |
| 7 | 2.5 | 2.7 | 5.2 | 1.117 | 40 | 40.10 | |
| 5 | 1.5 | 1.7 | 3.2 | 0.879 | 32 | 32.08 | |

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

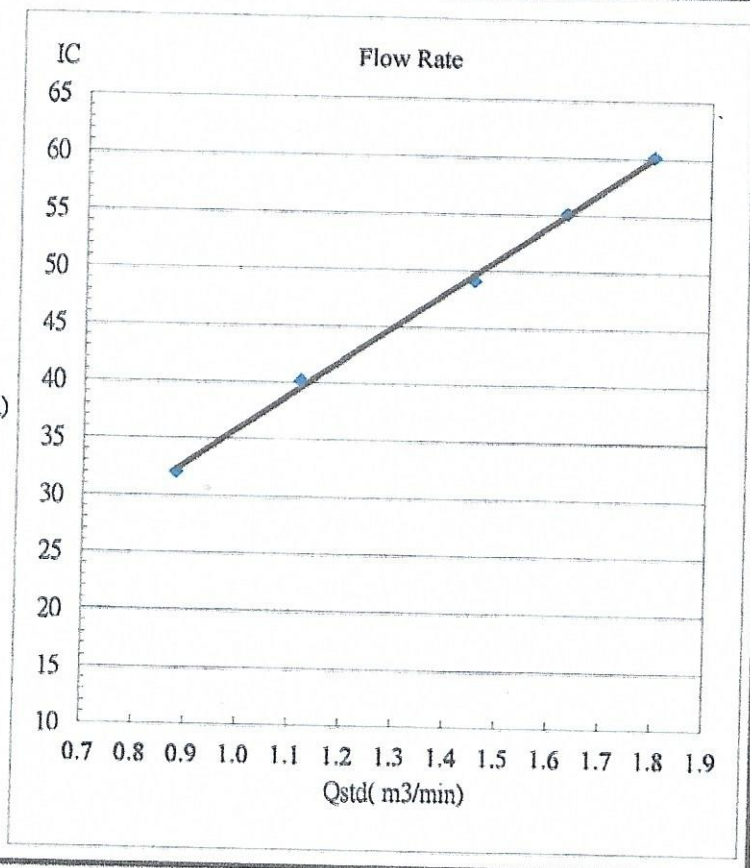



Certificate of Calibration

| Calibration Certification Information | | | |
|---------------------------------------|-----------------------------|-----------|-------|
| Cal. Date: December 15, 2023 | Rootsmeter S/N: 438320 | Ta: 295 | °K |
| Operator: Jim Tisch | | Pa: 748.5 | mm Hg |
| Calibration Model #: TE-5025A | Calibrator S/N: 2454 | | |


| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4250 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0090 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9040 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8610 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7110 | 12.8 | 8.00 |

| Data Tabulation | | | | | |
|-----------------|---------------|--|-----------|-------------|---|
| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis) |
| 0.9907 | 0.6952 | 1.4106 | 0.9957 | 0.6988 | 0.8878 |
| 0.9864 | 0.9776 | 1.9949 | 0.9914 | 0.9826 | 1.2556 |
| 0.9844 | 1.0890 | 2.2304 | 0.9894 | 1.0945 | 1.4037 |
| 0.9832 | 1.1420 | 2.3393 | 0.9882 | 1.1478 | 1.4723 |
| 0.9779 | 1.3754 | 2.8213 | 0.9829 | 1.3824 | 1.7756 |
| QSTD | m= | 2.07544 | QA | m= | 1.29961 |
| | b= | -0.03205 | | b= | -0.02017 |
| | r= | 0.99999 | | r= | 0.99999 |

| Calculations | |
|---|--|
| Vstd= $\Delta Vol \left(\frac{Pa - \Delta P}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)$ | Va= $\Delta Vol \left(\frac{Pa - \Delta P}{Pa} \right)$ |
| Qstd= Vstd/ΔTime | Qa= Va/ΔTime |
| For subsequent flow rate calculations: | |
| Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$ |

| Standard Conditions | |
|---------------------|---------------------------------------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: | calibrator manometer reading (in H2O) |
| ΔP: | rootsmeter manometer reading (mm Hg) |
| Ta: | actual absolute temperature (°K) |
| Pa: | actual barometric pressure (mm Hg) |
| b: | intercept |
| m: | slope |

| RECALIBRATION |
|--|
| US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30 |



Certificate of Calibration

校正證書

Certificate No. : C237046
證書編號

ITEM TESTED / 送檢項目 (Job No. / 序引編號 : IC23-2316) Date of Receipt / 收件日期 : 15 November 2023

Description / 儀器名稱 : Sound Level Meter
Manufacturer / 製造商 : Rion
Model No. / 型號 : NL-52
Serial No. / 編號 : 00175561
Supplied By / 委託者 : Envirotech Services Co.
Room 712, 7/F, My Loft, 9 Hoi Wing Road, Tuen Mun,
New Territories, Hong Kong

TEST CONDITIONS / 測試條件

Temperature / 溫度 : $(23 \pm 2)^{\circ}\text{C}$ Relative Humidity / 相對濕度 : $(50 \pm 25)\%$
Line Voltage / 電壓 : ---

TEST SPECIFICATIONS / 測試規範


Calibration check

DATE OF TEST / 測試日期 : 6 December 2023

TEST RESULTS / 測試結果

The results apply to the particular unit-under-test only.
The results do not exceed specified limits.
These limits refer to manufacturer's published tolerances as requested by the customer.
The results are detailed in the subsequent page(s).

The test equipment used for calibration are traceable to National Standards via :
- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory
- Hottinger Brüel & Kjær Calibration Laboratory, Denmark
- Agilent Technologies / Keysight Technologies
- Fluke Everett Service Center, USA

Tested By : 
測試 : _____
C K Lo
Project Engineer

Certified By : 
核證 : _____
K Q Lee
Engineer

Date of Issue : 6 December 2023
簽發日期

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗所書面批准。

Certificate of Calibration

校正證書

Certificate No. : C237046
證書編號

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 12 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- Self-calibration was performed before the test.
- The results presented are the mean of 3 measurements at each calibration point.
- Test equipment :

| Equipment ID | Description | Certificate No. |
|--------------|-------------------------------------|-----------------|
| CL280 | 40 MHz Arbitrary Waveform Generator | C230306 |
| CL281 | Multifunction Acoustic Calibrator | CDK2302738 |

- Test procedure : MA101N.

- Results :

6.1 Sound Pressure Level

6.1.1 Reference Sound Pressure Level

| UUT Setting | | | | Applied Value | | UUT Reading (dB) | IEC 61672 Class 1 Limit (dB) |
|-------------|----------------|---------------------|----------------|---------------|-------------|------------------|------------------------------|
| Range (dB) | Function | Frequency Weighting | Time Weighting | Level (dB) | Freq. (kHz) | | |
| 30 - 130 | L _A | A | Fast | 94.00 | 1 | 93.2 | ± 1.1 |

6.1.2 Linearity

| UUT Setting | | | | Applied Value | | UUT Reading (dB) |
|-------------|----------------|---------------------|----------------|---------------|-------------|------------------|
| Range (dB) | Function | Frequency Weighting | Time Weighting | Level (dB) | Freq. (kHz) | |
| 30 - 130 | L _A | A | Fast | 94.00 | 1 | 93.2 (Ref.) |
| | | | | 104.00 | | 103.3 |
| | | | | 114.00 | | 113.4 |

IEC 61672 Class 1 Limit : ± 0.6 dB per 10 dB step and ± 1.1 dB for overall different.

6.2 Time Weighting

| UUT Setting | | | | Applied Value | | UUT Reading (dB) | IEC 61672 Class 1 Limit (dB) |
|-------------|----------------|---------------------|----------------|---------------|-------------|------------------|------------------------------|
| Range (dB) | Function | Frequency Weighting | Time Weighting | Level (dB) | Freq. (kHz) | | |
| 30 - 130 | L _A | A | Fast | 94.00 | 1 | 93.2 | Ref. |
| | | | Slow | | | 93.2 | ± 0.3 |

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗所書面批准。

Certificate of Calibration

校正證書

Certificate No. : C237046
證書編號

6.3 Frequency Weighting

6.3.1 A-Weighting

| UUT Setting | | | | Applied Value | | UUT Reading (dB) | IEC 61672 Class 1 Limit (dB) |
|-------------|----------------|---------------------|----------------|---------------|--------|------------------|------------------------------|
| Range (dB) | Function | Frequency Weighting | Time Weighting | Level (dB) | Freq. | | |
| 30 - 130 | L _A | A | Fast | 94.00 | 63 Hz | 66.9 | -26.2 ± 1.5 |
| | | | | | 125 Hz | 77.0 | -16.1 ± 1.5 |
| | | | | | 250 Hz | 84.5 | -8.6 ± 1.4 |
| | | | | | 500 Hz | 89.9 | -3.2 ± 1.4 |
| | | | | | 1 kHz | 93.2 | Ref. |
| | | | | | 2 kHz | 94.4 | +1.2 ± 1.6 |
| | | | | | 4 kHz | 94.2 | +1.0 ± 1.6 |
| | | | | | 8 kHz | 92.1 | -1.1 (+2.1 ; -3.1) |
| | | | | | 16 kHz | 85.2 | -6.6 (+3.5 ; -17.0) |

6.3.2 C-Weighting

| UUT Setting | | | | Applied Value | | UUT Reading (dB) | IEC 61672 Class 1 Limit (dB) |
|-------------|----------------|---------------------|----------------|---------------|--------|------------------|------------------------------|
| Range (dB) | Function | Frequency Weighting | Time Weighting | Level (dB) | Freq. | | |
| 30 - 130 | L _C | C | Fast | 94.00 | 63 Hz | 92.3 | -0.8 ± 1.5 |
| | | | | | 125 Hz | 93.0 | -0.2 ± 1.5 |
| | | | | | 250 Hz | 93.2 | 0.0 ± 1.4 |
| | | | | | 500 Hz | 93.2 | 0.0 ± 1.4 |
| | | | | | 1 kHz | 93.2 | Ref. |
| | | | | | 2 kHz | 93.0 | -0.2 ± 1.6 |
| | | | | | 4 kHz | 92.4 | -0.8 ± 1.6 |
| | | | | | 8 kHz | 90.2 | -3.0 (+2.1 ; -3.1) |
| | | | | | 16 kHz | 83.3 | -8.5 (+3.5 ; -17.0) |

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室所書面批准。



Certificate of Calibration

校正證書

Certificate No. : C237046
證書編號

Remarks : - UUT Microphone Model No. : UC-59 & S/N : 16651

- Mfr's Limit : IEC 61672 Class 1

- Uncertainties of Applied Value :

| | | |
|--------|------------------|--------------------------|
| 94 dB | : 63 Hz - 125 Hz | : ± 0.35 dB |
| | 250 Hz - 500 Hz | : ± 0.30 dB |
| | 1 kHz | : ± 0.20 dB |
| | 2 kHz - 4 kHz | : ± 0.35 dB |
| | 8 kHz | : ± 0.45 dB |
| | 16 kHz | : ± 0.70 dB |
| 104 dB | : 1 kHz | : ± 0.10 dB (Ref. 94 dB) |
| 114 dB | : 1 kHz | : ± 0.10 dB (Ref. 94 dB) |

- The uncertainties are for a confidence probability of not less than 95 %.

Note :

Only the original copy or the laboratory's certified true copy is valid.

The values given in this Certificate only relate to the values measured at the time of the test and any uncertainties quoted will not include allowance for the equipment long term drift, variations with environment changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the measurement. Sun Creation Engineering Limited shall not be liable for any loss or damage resulting from the use of the equipment.

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室書面批准。



Certificate of Calibration 校正證書

Certificate No. : C242738
證書編號

ITEM TESTED / 送檢項目 (Job No. / 序引編號 : IC24-0781)

Date of Receipt / 收件日期 : 3 May 2024

Description / 儀器名稱 : Precision Acoustic Calibrator
Manufacturer / 製造商 : LARSON DAVIS
Model No. / 型號 : CAL200
Serial No. / 編號 : 11334
Supplied By / 委託者 : Envirotech Services Co.
Room 712, 7/F, My Loft, 9 Hoi Wing Road, Tuen Mun,
New Territories, Hong Kong

TEST CONDITIONS / 測試條件

Temperature / 溫度 : $(23 \pm 2)^{\circ}\text{C}$
Line Voltage / 電壓 : ---

Relative Humidity / 相對濕度 : $(50 \pm 25)\%$

TEST SPECIFICATIONS / 測試規範


Calibration check

DATE OF TEST / 測試日期 : 19 May 2024

TEST RESULTS / 測試結果

The results apply to the particular unit-under-test only.
The results do not exceed specified limits.
These limits refer to manufacturer's published or user's specified tolerances as requested by the customer.
The results are detailed in the subsequent page(s).


The test equipment used for calibration are traceable to National Standards via :
- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory
- Hottinger Brüel & Kjær Calibration Laboratory, Denmark
- Agilent Technologies / Keysight Technologies
- Fluke Everett Service Center, USA

Tested By : 
測試 : H T Wong
Assistant Engineer

Certified By : 
核證 : K C Lee
Engineer

Date of Issue : 20 May 2024
簽發日期

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.
本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室書面批准。



Certificate of Calibration

校正證書

Certificate No. : C242738
證書編號

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 12 hours before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.
- Test equipment :

| <u>Equipment ID</u> | <u>Description</u> | <u>Certificate No.</u> |
|---------------------|-----------------------------------|------------------------|
| CL130 | Universal Counter | C233799 |
| CL281 | Multifunction Acoustic Calibrator | CDK2302738 |
| TST150A | Measuring Amplifier | C241879 |

- Test procedure : MA100N.

- Results :

5.1 Sound Level Accuracy

| UUT Nominal Value | Measured Value (dB) | User's Limit (dB) | Uncertainty of Measured Value (dB) |
|-------------------|---------------------|-------------------|------------------------------------|
| 94 dB, 1 kHz | 93.60 | ± 0.5 | ± 0.20 |
| 114 dB, 1 kHz | 113.60 | | |

5.2 Frequency Accuracy

| UUT Nominal Value (kHz) | Measured Value (kHz) | Mfr's Limit | Uncertainty of Measured Value (Hz) |
|-------------------------|----------------------|-------------|------------------------------------|
| 1 | 1.000 | 1 kHz ± 1 % | ± 1 |

Remarks : - The user's limit is a customer pre-defined operating tolerance of the UUT, suitable for one's own intended use.

- The uncertainties are for a confidence probability of not less than 95 %.

Note :

Only the original copy or the laboratory's certified true copy is valid.

The values given in this Certificate only relate to the values measured at the time of the test and any uncertainties quoted will not include allowance for the equipment long term drift, variations with environment changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the measurement. Sun Creation Engineering Limited shall not be liable for any loss or damage resulting from the use of the equipment.

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室書面批准。