

High-Volume TSP Sampler  
5-Point Calibration Record

Location : AM1(ICC)  
Calibrated by : K.T.Ho  
Date : 05/03/2025

Sampler

Model : TE-5170  
Serial Number : S/N 0767

Calibration Orifice and Standard Calibration Relationship

Serial Number : 2454  
Next Calibration Date : 02 December 2025  
Slope (m) : 2.08315  
Intercept (b) : -0.04938  
Correlation Coefficient(r) : 0.99985

Standard Condition

Pstd (hpa) : 1013  
Tstd (K) : 298.18

Calibration Condition


Pa (hpa) : 1013  
Ta(K) : 295

| Resistance Plate |          | dH [green liquid]<br>(inch water) | Z     | X=Qstd<br>(cubic meter/min) | IC<br>(chart) | Y<br>(corrected) |
|------------------|----------|-----------------------------------|-------|-----------------------------|---------------|------------------|
| 1                | 18 holes | 11.2                              | 3.364 | 1.639                       | 58            | 58.30            |
| 2                | 13 holes | 8.2                               | 2.878 | 1.405                       | 50            | 50.26            |
| 3                | 10 holes | 6.2                               | 2.503 | 1.225                       | 42            | 42.22            |
| 4                | 7 holes  | 4.4                               | 2.109 | 1.036                       | 34            | 34.18            |
| 5                | 5 holes  | 2.6                               | 1.621 | 0.802                       | 22            | 22.11            |

Notes:  $Z = \sqrt{\frac{dH(Pa/Pstd)(Tstd/Ta)}{}}$ ,  $X = Z/m - b$ ,  $Y(\text{Corrected Flow}) = IC * \{\sqrt{\frac{Pa(Pa/Pstd)(Tstd/Ta)}{}}\}$

Sampler Calibration Relationship

Slope(m): 43.298      Intercept(b): -11.470      Correlation Coefficient(r): 0.9972

Checked by:   
Magnum Fan

Date: 08/03/2025

# Certificate of Calibration

**Calibration Certification Information**
**Cal. Date:** December 2, 2024

**Rootsmeter S/N:** 438320

**Ta:** 293

**°K**
**Operator:** Jim Tisch

**Pa:** 757.4

**mm Hg**
**Calibration Model #:** TE-5025A

**Calibrator S/N:** 2454

| Run | Vol. Init<br>(m3) | Vol. Final<br>(m3) | ΔVol.<br>(m3) | ΔTime<br>(min) | ΔP<br>(mm Hg) | ΔH<br>(in H2O) |
|-----|-------------------|--------------------|---------------|----------------|---------------|----------------|
| 1   | 1                 | 2                  | 1             | 1.4200         | 3.2           | 2.00           |
| 2   | 3                 | 4                  | 1             | 1.0170         | 6.4           | 4.00           |
| 3   | 5                 | 6                  | 1             | 0.9090         | 7.9           | 5.00           |
| 4   | 7                 | 8                  | 1             | 0.8700         | 8.8           | 5.50           |
| 5   | 9                 | 10                 | 1             | 0.7140         | 12.8          | 8.00           |

**Data Tabulation**

| Vstd<br>(m3) | Qstd<br>(x-axis) | $\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$<br>(y-axis) | Va        | Qa<br>(x-axis) | $\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$<br>(y-axis) |
|--------------|------------------|---|-----------|----------------|--|
| 1.0093       | 0.7108           | 1.4238  | 0.9958    | 0.7013         | 0.8796   |
| 1.0051       | 0.9883           | 2.0136  | 0.9916    | 0.9750         | 1.2439   |
| 1.0031       | 1.1035           | 2.2512  | 0.9896    | 1.0886         | 1.3907   |
| 1.0018       | 1.1515           | 2.3611  | 0.9884    | 1.1361         | 1.4586   |
| 0.9965       | 1.3956           | 2.8476  | 0.9831    | 1.3769         | 1.7592   |
| <b>QSTD</b>  | <b>m=</b>        | <b>2.08315</b>  | <b>QA</b> | <b>m=</b>      | <b>1.30443</b>   |
|              | <b>b=</b>        | <b>-0.04938</b>   |           | <b>b=</b>      | <b>-0.03050</b>  |
|              | <b>r=</b>        | <b>0.99985</b>  |           | <b>r=</b>      | <b>0.99985</b>   |

**Calculations**

|  |   |   |                                |
|--|---|---|--------------------------------|
| <b>Vstd=</b>   | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$ | <b>Va=</b>  | $\Delta Vol((Pa-\Delta P)/Pa)$ |
| <b>Qstd=</b>   | $Vstd/\Delta Time$                        | <b>Qa=</b>  | $Va/\Delta Time$               |
| <b>For subsequent flow rate calculations:</b>  |   |   |                                |
| <b>Qstd=</b> $1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$ |   | <b>Qa=</b> $1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$ |                                |

**Standard Conditions**

|   |           |
|---|-----------|
| <b>Tstd:</b>                              | 298.15 °K |
| <b>Pstd:</b>                              | 760 mm Hg |
| <b>Key</b>                                |           |
| ΔH: calibrator manometer reading (in H2O) |           |
| ΔP: rootsmeter manometer reading (mm Hg)  |           |
| Ta: actual absolute temperature (°K)      |           |
| Pa: actual barometric pressure (mm Hg)    |           |
| b: intercept                              |           |
| m: slope                                  |           |

**RECALIBRATION**

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



### SUB-CONTRACTING REPORT

CONTACT : MR MAGNUM FAN

CLIENT : ENVIROTECH SERVICES CO.

ADDRESS : RM 712, 7/F, MY LOFT 9 HOI WING ROAD,  
TUEN MUN, N.T. HK

PROJECT :

WORK ORDER : HK2417958

SUB-BATCH : 1

DATE RECEIVED : 8-MAY-2024

DATE OF ISSUE : 14-MAY-2024

NO. OF SAMPLES : 1

CLIENT ORDER :

#### General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
- Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
- Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
- Calibration was subcontracted to Envirotech Services Company.

#### Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

**ALS Technichem (HK) Pty Ltd**  
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong  
Tel. +852 2610 1044 Fax +852 2610 2021 [www.alsglobal.com](http://www.alsglobal.com)

WORK ORDER : HK2417958  
SUB-BATCH : 1  
CLIENT : ENVIROTECH SERVICES CO.  
PROJECT : ----



| ALS Lab ID    | Client's Sample ID    | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2417958-001 | Sibata LD 5R (841724) | Equipments  | 30-Apr-2024 | S/N: 841724             |





Envirotech Services Co.

Rm. 712, 7/F  
My Loft,  
9 Hoi Wing Road,  
Tuen Mun, H.K.  
Tel : 2660 8450  
Fax : 2660 8553  
E mail: envirotech@envirotech.com

### Equipment Verification Report (TSP)

#### Equipment Calibrated:

Type: Laser Dust Monitor  
Manufacturer: Sibata LD-5R  
Serial No.: 841724  
Equipment Ref.: N/A  
ALS Job Order: HK2416892

#### Standard Equipment

Standard Equipment: High Volume Sampler (TSP)  
Location: Envirotech Room (Calibration Room)  
Equipment Ref.: HVS 8162  
Last Calibration Date: 25-Mar-2024


#### Equipment Verification Results:

Verification Date: 30-Apr-2024

| Hour       | Time      | Mean Temp °C | Mean Pressure (hpa) | Concentration in $\mu\text{g}/\text{m}^3$ (Standard Equipment) (Y-Axis) | Concentration in $\mu\text{g}/\text{m}^3$ (Calibrated Equipment) (X-Axis) |
|------------|-----------|--------------|---------------------|---|---|
| 1hr 00mins | 0845-0945 | 28.5         | 1005                | 32  | 25  |
| 2hr 00mins | 0950-1150 | 28.5         | 1005                | 66  | 54  |
| 3hr 00mins | 1315-1615 | 29.6         | 1005                | 93  | 75  |

#### Linear Regression of Y or X

Slope (K-factor):  $1.2312(\mu\text{g}/\text{m}^3)/\text{CPM}$   
Correlation Coefficient (R): 0.9999  
Date of Issue: 8-May-2024

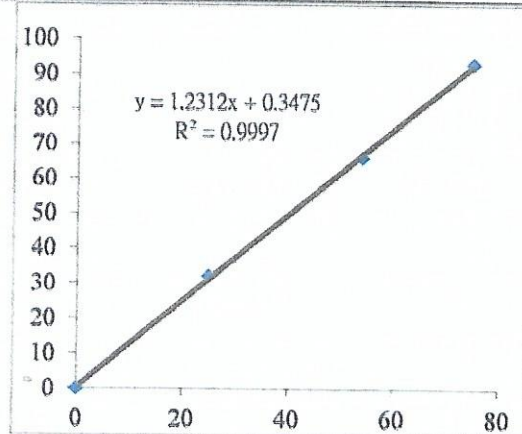

#### Remarks:

1. Strong Correlation ( $>0.8$ )
2. Factor  $1.2312(\mu\text{g}/\text{m}^3)/\text{CPM}$  should be applied for TSP monitoring

\*If  $R < 0.5$ , repair or verification is required for the equipment

Operator: P.F.Yeung Signature Tai Date: 08 May 2024

QC Reviewer: K.F.Ho Signature at Date: 08 May 2024

# TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location : Rm. 712, My Loft, Tuen Mun

HVS ID: 8162

Name and Model : TISCH HVS Model TE-5170

Date of Calibration:

25-Mar-24

Next Calibration Date:

24-May-24

Operator:

P.F. Yeung

## CONDITIONS

Sea Level Pressure (hpa)

1016

Temperature (°C)

24.5

Corrected Pressure (mm Hg)

762.1

Temperature (K)

297.5

## CALIBRATION ORIFICE

Make:

TISCH

Model:

TE-5025A

Serial#:

2454

Qstd Slope

2.07544

Qstd Intercept

-0.03205

## CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION   |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|---|
| 18        | 6.7         | 6.8         | 13.5     | 1.790         | 60        | 60.15          | Slope= 30.471<br>Intercept= 5.514<br>Corr. Coeff.= 0.9994 |
| 13        | 5.5         | 5.6         | 11.1     | 1.625         | 55        | 55.13          |   |
| 10        | 4.3         | 4.5         | 8.8      | 1.448         | 49        | 49.12          |   |
| 7         | 2.5         | 2.7         | 5.2      | 1.117         | 40        | 40.10          |   |
| 5         | 1.5         | 1.7         | 3.2      | 0.879         | 32        | 32.08          |   |

### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

### For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

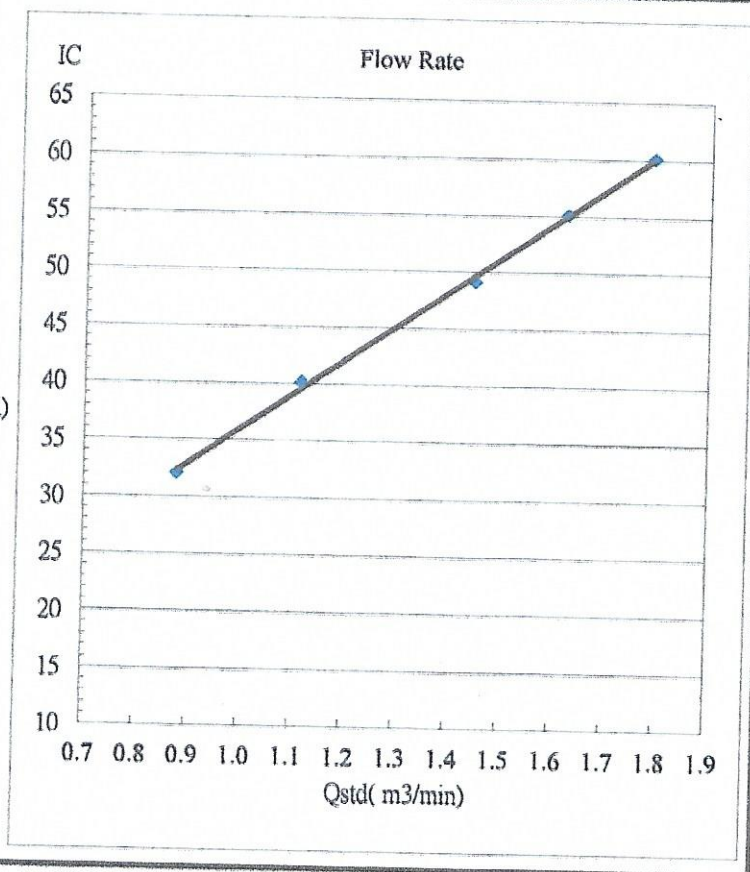



## Certificate of Calibration

### Calibration Certification Information

|                               |                             |                 |
|-------------------------------|-----------------------------|-----------------|
| Cal. Date: December 15, 2023  | Rootsmeter S/N: 438320      | Ta: 295 °K      |
| Operator: Jim Tisch           |                             | Pa: 748.5 mm Hg |
| Calibration Model #: TE-5025A | Calibrator S/N: <b>2454</b> |                 |

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1   | 1              | 2               | 1          | 1.4250      | 3.2        | 2.00        |
| 2   | 3              | 4               | 1          | 1.0090      | 6.4        | 4.00        |
| 3   | 5              | 6               | 1          | 0.9040      | 7.9        | 5.00        |
| 4   | 7              | 8               | 1          | 0.8610      | 8.8        | 5.50        |
| 5   | 9              | 10              | 1          | 0.7110      | 12.8       | 8.00        |

### Data Tabulation

| Vstd (m3)   | Qstd (x-axis) | $\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis) | Va        | Qa (x-axis) | $\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$ (y-axis) |
|-------------|---------------|--|-----------|-------------|---|
| 0.9907      | 0.6952        | 1.4106   | 0.9957    | 0.6988      | 0.8878  |
| 0.9864      | 0.9776        | 1.9949   | 0.9914    | 0.9826      | 1.2556  |
| 0.9844      | 1.0890        | 2.2304   | 0.9894    | 1.0945      | 1.4037  |
| 0.9832      | 1.1420        | 2.3393   | 0.9882    | 1.1478      | 1.4723  |
| 0.9779      | 1.3754        | 2.8213   | 0.9829    | 1.3824      | 1.7756  |
| <b>QSTD</b> | m=            | <b>2.07544</b>   | <b>QA</b> | m=          | <b>1.29961</b>  |
|             | b=            | <b>-0.03205</b>  |           | b=          | <b>-0.02017</b>   |
|             | r=            | <b>0.99999</b>   |           | r=          | <b>0.99999</b>  |

### Calculations

|   |   |  |                                |
|---|---|--|--------------------------------|
| Vstd=   | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$ | Va=  | $\Delta Vol((Pa-\Delta P)/Pa)$ |
| Qstd=   | Vstd/ΔTime                                | Qa=  | Va/ΔTime                       |
| For subsequent flow rate calculations:  |   |  |                                |
| Qstd= $1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$ |   | Qa= $1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$ |                                |

### Standard Conditions

|   |           |
|---|-----------|
| Tstd:                                     | 298.15 °K |
| Pstd:                                     | 760 mm Hg |
| <b>Key</b>                                |           |
| ΔH: calibrator manometer reading (in H2O) |           |
| ΔP: rootsmeter manometer reading (mm Hg)  |           |
| Ta: actual absolute temperature (°K)      |           |
| Pa: actual barometric pressure (mm Hg)    |           |
| b: intercept                              |           |
| m: slope                                  |           |

### RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



### SUB-CONTRACTING REPORT

|         |  |                |               |
|---------|--|----------------|---------------|
| CONTACT | : MR MAGNUM FAN  | WORK ORDER     | : HK2419604   |
| CLIENT  | : ENVIROTECH SERVICES CO.                                    |                |               |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD,<br>TUEN MUN, N.T. HK | SUB-BATCH      | : 1           |
|         |  | DATE RECEIVED  | : 20-MAY-2024 |
|         |  | DATE OF ISSUE  | : 24-MAY-2024 |
| PROJECT | : ----   | NO. OF SAMPLES | : 1           |
|         |  | CLIENT ORDER   | : ----        |

### General Comments

- Sample Information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
- Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
- Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
- Calibration was subcontracted to Envirotech Services Company.

### Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

**ALS Technichem (HK) Pty Ltd**  
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong  
Tel. +852 2610 1044 Fax +852 2610 2021 [www.alsglobal.com](http://www.alsglobal.com)



WORK ORDER : HK2419604  
SUB-BATCH : 1  
CLIENT : ENVIROTECH SERVICES CO.  
PROJECT :



| ALS Lab ID    | Client's Sample ID    | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2419604-001 | Sibata LD-3B (235786) | Equipments  | 11-May-2024 | S/N: 235786             |

----- END OF REPORT -----



Envirotech Services Co.

Rm. 712, 7/F  
My Loft,  
9 Hoi Wing Road,  
Tuen Mun, H.K.  
Tel : 2660 8460  
Fax : 2660 8553  
E-mail: [envirotech@netvigator.com](mailto:envirotech@netvigator.com)

## Equipment Verification Report (TSP)

### Equipment Calibrated:

Type: Laser Dust Monitor  
Manufacturer: Sibata LD-3B  
Serial No.: 235786  
Equipment Ref.: N/A  
ALS Job Order: HK2418944

### Standard Equipment

Standard Equipment: High Volume Sampler (TSP)  
Location: Envirotech Room (Calibration Room)  
Equipment Ref.: HVS 8162  
Last Calibration Date: 25-Mar-2024


### Equipment Verification Results:

Verification Date: 11-May-2024

| Hour       | Time      | Mean Temp °C | Mean Pressure (hpa) | Concentration in $\mu\text{g}/\text{m}^3$ (Standard Equipment) (Y-Axis) | Concentration in $\mu\text{g}/\text{m}^3$ (Calibrated Equipment) (X-Axis) |
|------------|-----------|--------------|---------------------|---|---|
| 1hr 00mins | 0830-0930 | 26.8         | 1015                | 34  | 28  |
| 2hr 00mins | 0935-1135 | 28.5         | 1015                | 53  | 48  |
| 3hr 00mins | 1310-1610 | 29.5         | 1016                | 133   | 105   |

### Linear Regression of Y or X

Slope (K-factor):  $1.2673(\mu\text{g}/\text{m}^3)/\text{CPM}$   
Correlation Coefficient (R): 0.9978  
Date of Issue: 19-May-2024

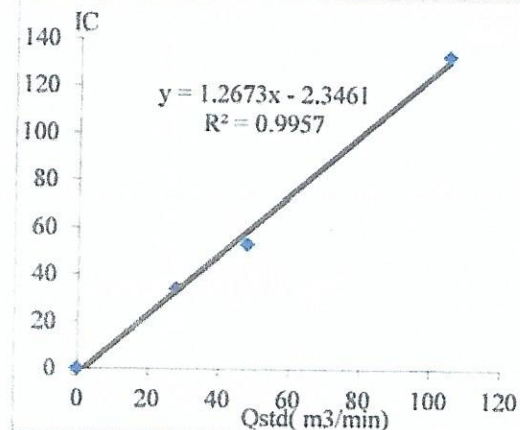

### Remarks:

1. Strong Correlation ( $>0.8$ )
2. Factor  $1.2673(\mu\text{g}/\text{m}^3)/\text{CPM}$  should be applied for TSP monitoring

\*If  $R < 0.5$ , repair or verification is required for the equipment

Operator: P.F.Yeung Signature Tai Date: 19 May 2024

QC Reviewer: K.F.Ho Signature at Date: 19 May 2024

# TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location : Rm. 712, My Loft, Tuen Mun

HVS ID: 8162

Name and Model : TISCH HVS Model TE-5170

Date of Calibration:

25-Mar-24

Next Calibration Date:

24-May-24

Operator:

P.F. Yeung

## CONDITIONS

Sea Level Pressure (hpa)

1016

Temperature (°C)

24.5

Corrected Pressure (mm Hg)

762.1

Temperature (K)

297.5

## CALIBRATION ORIFICE

Make:

TISCH

Model:

TE-5025A

Serial#:

2454

Qstd Slope

2.07544

Qstd Intercept

-0.03205

## CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION   |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|---|
| 18        | 6.7         | 6.8         | 13.5     | 1.790         | 60        | 60.15          | Slope= 30.471<br>Intercept= 5.514<br>Corr. Coeff.= 0.9994 |
| 13        | 5.5         | 5.6         | 11.1     | 1.625         | 55        | 55.13          |   |
| 10        | 4.3         | 4.5         | 8.8      | 1.448         | 49        | 49.12          |   |
| 7         | 2.5         | 2.7         | 5.2      | 1.117         | 40        | 40.10          |   |
| 5         | 1.5         | 1.7         | 3.2      | 0.879         | 32        | 32.08          |   |

### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

### For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

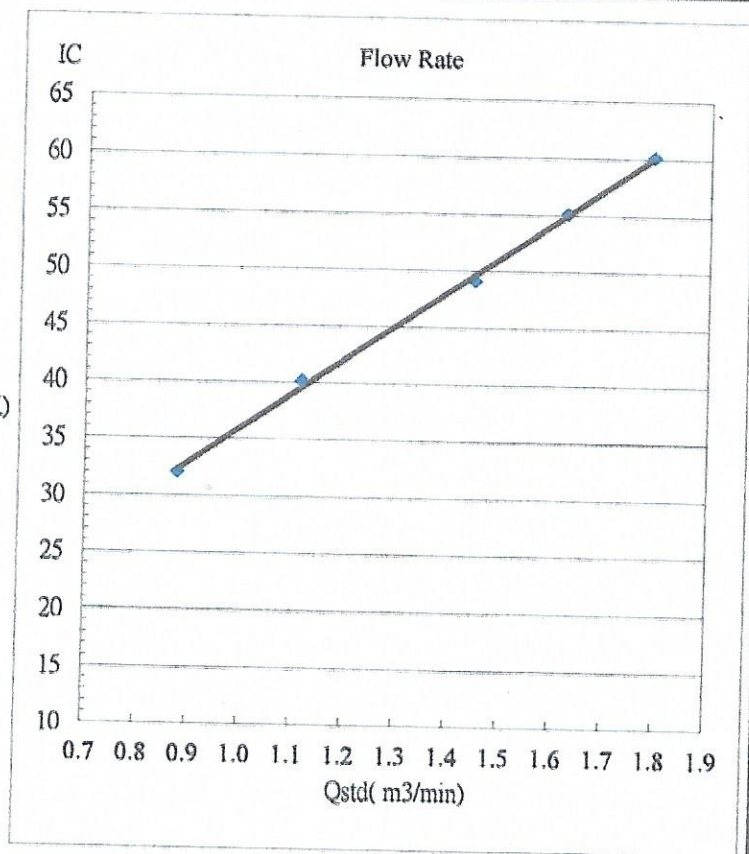





# Certificate of Calibration

## Calibration Certification Information

Cal. Date: December 15, 2023      Rootsmeter S/N: 438320      Ta: 295 °K  
Operator: Jim Tisch      Pa: 748.5 mm Hg  
Calibration Model #: TE-5025A      Calibrator S/N: **2454**

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1   | 1              | 2               | 1          | 1.4250      | 3.2        | 2.00        |
| 2   | 3              | 4               | 1          | 1.0090      | 6.4        | 4.00        |
| 3   | 5              | 6               | 1          | 0.9040      | 7.9        | 5.00        |
| 4   | 7              | 8               | 1          | 0.8610      | 8.8        | 5.50        |
| 5   | 9              | 10              | 1          | 0.7110      | 12.8       | 8.00        |

## Data Tabulation

| Vstd (m3)   | Qstd (x-axis) | $\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis) | Va        | Qa (x-axis) | $\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$ (y-axis) |
|-------------|---------------|--|-----------|-------------|---|
| 0.9907      | 0.6952        | 1.4106   | 0.9957    | 0.6988      | 0.8878  |
| 0.9864      | 0.9776        | 1.9949   | 0.9914    | 0.9826      | 1.2556  |
| 0.9844      | 1.0890        | 2.2304   | 0.9894    | 1.0945      | 1.4037  |
| 0.9832      | 1.1420        | 2.3393   | 0.9882    | 1.1478      | 1.4723  |
| 0.9779      | 1.3754        | 2.8213   | 0.9829    | 1.3824      | 1.7756  |
| <b>QSTD</b> | m=            | <b>2.07544</b>   | <b>QA</b> | m=          | <b>1.29961</b>  |
|             | b=            | <b>-0.03205</b>  |           | b=          | <b>-0.02017</b>   |
|             | r=            | <b>0.99999</b>   |           | r=          | <b>0.99999</b>  |

## Calculations

|  |   |
|--|---|
| <b>Vstd=</b> $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$   | <b>Va=</b> $\Delta Vol((Pa-\Delta P)/Pa)$   |
| <b>Qstd=</b> $Vstd/\Delta Time$  | <b>Qa=</b> $Va/\Delta Time$   |
| <b>For subsequent flow rate calculations:</b>  |   |
| <b>Qstd=</b> $1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$ | <b>Qa=</b> $1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$ |

## Standard Conditions

|   |           |
|---|-----------|
| Tstd:                                     | 298.15 °K |
| Pstd:                                     | 760 mm Hg |
| <b>Key</b>                                |           |
| ΔH: calibrator manometer reading (in H2O) |           |
| ΔP: rootsmeter manometer reading (mm Hg)  |           |
| Ta: actual absolute temperature (°K)      |           |
| Pa: actual barometric pressure (mm Hg)    |           |
| b: intercept                              |           |
| m: slope                                  |           |

## RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30





### SUB-CONTRACTING REPORT

|         |  |                |                    |
|---------|--|----------------|--------------------|
| CONTACT | : MR MAGNUM FAN  | WORK ORDER     | : <b>HK2448121</b> |
| CLIENT  | : ENVIROTECH SERVICES CO.                                    |                |                    |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD,<br>TUEN MUN, N.T. HK | SUB-BATCH      | : 1                |
|         |  | DATE RECEIVED  | : 13-NOV-2024      |
|         |  | DATE OF ISSUE  | : 20-NOV-2024      |
| PROJECT | : ----   | NO. OF SAMPLES | : 1                |
|         |  | CLIENT ORDER   | : ----             |

#### General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
- Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
- Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
- Calibration was subcontracted to Envirotech Services Company.

#### Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

*Signatories*

*Position*

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

**ALS Technichem (HK) Pty Ltd**  
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong  
Tel. +852 2610 1044 Fax. +852 2610 2021 [www.alsglobal.com](http://www.alsglobal.com)

WORK ORDER : HK2448121  
SUB-BATCH : 1  
CLIENT : ENVIROTECH SERVICES CO.  
PROJECT : ----



| ALS Lab ID    | Client's Sample ID    | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2448121-001 | Sibata LD-3B (245834) | Equipments  | 09-Nov-2024 | S/N: 245834             |

----- END OF REPORT -----



Envirotech Services Co.

Rm. 712, 7/F  
My Loft,  
9 Hoi Wing Road,  
Tuen Mun, H.K.  
Tel : 2560 8450  
Fax : 2560 8553  
E-mail: envirotech@netvigator.com

## Equipment Verification Report (TSP)

### Equipment Calibrated:

Type: Laser Dust Monitor  
Manufacturer: Sibata LD-3B  
Serial No.: 245834  
Equipment Ref.: N/A  
ALS Job Order: HK2446853

### Standard Equipment

Standard Equipment: High Volume Sampler (TSP)  
Location: Envirotech Room (Calibration Room)  
Equipment Ref.: HVS 8162  
Last Calibration Date: 19-Oct-2024


### Equipment Verification Results:

Verification Date: 9-Nov-2024

| Hour       | Time      | Mean Temp °C | Mean Pressure (hpa) | Concentration in $\mu\text{g}/\text{m}^3$ (Standard Equipment) (Y-Axis) | Concentration in $\mu\text{g}/\text{m}^3$ (Calibrated Equipment) (X-Axis) |
|------------|-----------|--------------|---------------------|---|---|
| 1hr 00mins | 0905-1005 | 24.9         | 1013                | 85  | 104   |
| 2hr 00mins | 1015-1215 | 25.2         | 1014                | 155   | 193   |
| 3hr 00mins | 1430-1730 | 25.6         | 1014                | 196   | 250   |

### Linear Regression of Y or X

Slope (K-factor):  $1.2705(\mu\text{g}/\text{m}^3)/\text{CPM}$   
Correlation Coefficient (R): 0.9997  
Date of Issue: 13-Nov-2024

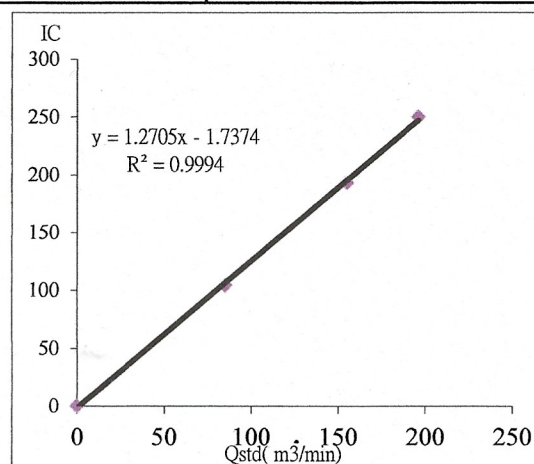

### Remarks:

1. Strong Correlation ( $>0.8$ )
2. Factor  $1.2705(\mu\text{g}/\text{m}^3)/\text{CPM}$  should be applied for TSP monitoring

\*If  $R < 0.5$ , repair or verification is required for the equipment

Operator: P.F.Yeung Signature: Date: 11 Nov 2024

QC Reviewer: K.F.Ho Signature: Date: 11 Nov 2024

## TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location : Rm. 712, My Loft, Tuen Mun      Date of Calibration: 19-Oct-24  
HVS ID: 8162      Next Calibration Date: 19-Dec-24  
Name and Model : TISCH HVS Model TE-5170      Operator: K.F.Ho

### CONDITIONS

|                          |      |                            |       |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1015 | Corrected Pressure (mm Hg) | 761.3 |
| Temperature (°C)         | 26.0 | Temperature (K)            | 299   |

### CALIBRATION ORIFICE

|          |          |                |          |
|----------|----------|----------------|----------|
| Make:    | TISCH    | Qstd Slope     | 2.07544  |
| Model:   | TE-5025A | Qstd Intercept | -0.03205 |
| Serial#: | 2454     |                |          |

### CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION  |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|--|
| 18        | 6.1         | 6.4         | 12.5     | 1.718         | 62        | 61.97          | Slope= 45.67<br>Intercept= -15.103<br>Corr. Coeff.= 0.9947 |
| 13        | 4.9         | 5.2         | 10.1     | 1.546         | 56        | 55.97          |  |
| 10        | 3.6         | 3.8         | 7.4      | 1.325         | 48        | 47.97          |  |
| 7         | 2.4         | 2.7         | 5.1      | 1.103         | 34        | 33.98          |  |
| 5         | 1.4         | 1.7         | 3.1      | 0.863         | 24        | 23.99          |  |

#### Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

#### For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

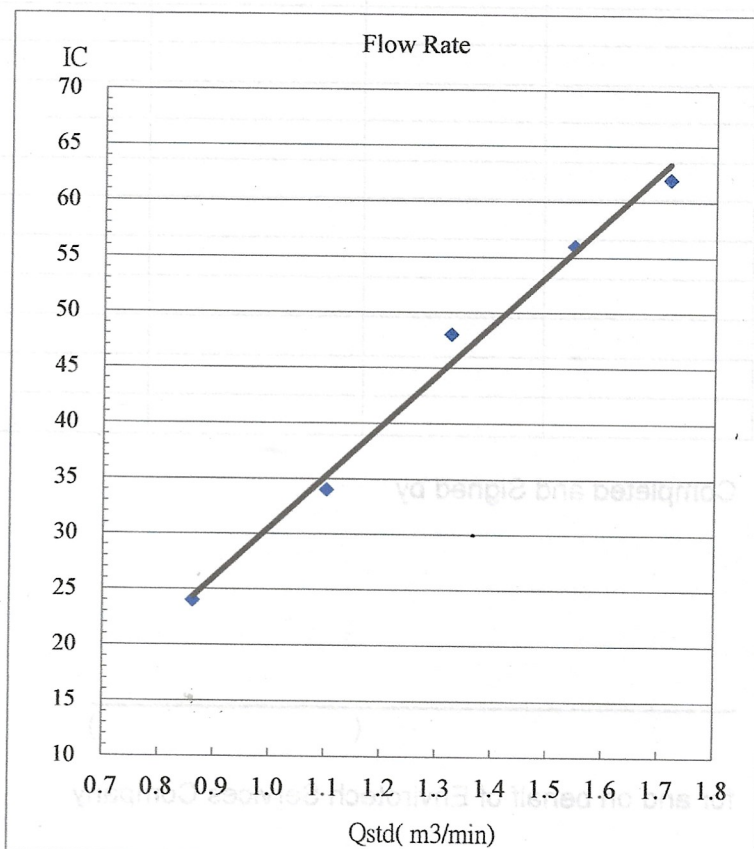



## Certificate of Calibration

### Calibration Certification Information

Cal. Date: December 15, 2023      Rootsmeter S/N: 438320      Ta: 295 °K  
 Operator: Jim Tisch      Pa: 748.5 mm Hg  
 Calibration Model #: TE-5025A      Calibrator S/N: 2454

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1   | 1              | 2               | 1          | 1.4250      | 3.2        | 2.00        |
| 2   | 3              | 4               | 1          | 1.0090      | 6.4        | 4.00        |
| 3   | 5              | 6               | 1          | 0.9040      | 7.9        | 5.00        |
| 4   | 7              | 8               | 1          | 0.8610      | 8.8        | 5.50        |
| 5   | 9              | 10              | 1          | 0.7110      | 12.8       | 8.00        |

### Data Tabulation

| Vstd (m3)   | Qstd (x-axis) | $\sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)}$ (y-axis) | Va        | Qa (x-axis) | $\sqrt{\Delta H \left( \frac{Ta}{Pa} \right)}$ (y-axis) |
|-------------|---------------|--|-----------|-------------|---|
| 0.9907      | 0.6952        | 1.4106   | 0.9957    | 0.6988      | 0.8878  |
| 0.9864      | 0.9776        | 1.9949   | 0.9914    | 0.9826      | 1.2556  |
| 0.9844      | 1.0890        | 2.2304   | 0.9894    | 1.0945      | 1.4037  |
| 0.9832      | 1.1420        | 2.3393   | 0.9882    | 1.1478      | 1.4723  |
| 0.9779      | 1.3754        | 2.8213   | 0.9829    | 1.3824      | 1.7756  |
| <b>QSTD</b> | m=            | <b>2.07544</b>   | <b>QA</b> | m=          | <b>1.29961</b>  |
|             | b=            | <b>-0.03205</b>  |           | b=          | <b>-0.02017</b>   |
|             | r=            | <b>0.99999</b>   |           | r=          | <b>0.99999</b>  |

### Calculations

|  |   |     |  |
|--|---|-----|--|
| Vstd=                                  | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$   | Va= | $\Delta Vol((Pa-\Delta P)/Pa)$   |
| Qstd=                                  | Vstd/ΔTime  | Qa= | Va/ΔTime   |
| For subsequent flow rate calculations: |   |     |  |
| Qstd=                                  | $1/m \left( \left( \sqrt{\Delta H \left( \frac{Pa}{Pstd} \right) \left( \frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= | $1/m \left( \left( \sqrt{\Delta H \left( \frac{Ta}{Pa} \right)} \right) - b \right)$ |

### Standard Conditions

Tstd: 298.15 °K

Pstd: 760 mm Hg

### Key

ΔH: calibrator manometer reading (in H2O)

ΔP: rootsmeter manometer reading (mm Hg)

Ta: actual absolute temperature (°K)

Pa: actual barometric pressure (mm Hg)

b: intercept

m: slope

### RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

# *Certificate of Calibration*

*for*

*Description:* **Sound Level Meter**  
*Manufacturer:* **RION**  
*Type No.:* **NL-52 (Serial No.: 00643040)**  
*Microphone:* **PCB 377B02 (Serial No.: 172764)**  
*Preamplifier:* **NH-25 (Serial No.: 21757)**

***Submitted by:***

*Customer:* **Envirotech Services Co.**  
*Address:* **Rm. 712, 7/F., My Loft, 9 Hoi Wing Road,  
Tuen Mun, Hong Kong**

**Upon receipt for calibration, the instrument was found to be:**

- ☒ **Within (31.5Hz – 8kHz)**  
☐ **Outside**

**the allowable tolerance.**

The test equipment used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

**Date of receipt: 25 September 2024**

**Date of calibration: 27 September 2024**

**Date of NEXT calibration: 26 September 2025**

**Calibrated by:**   
**Calibration Technician**

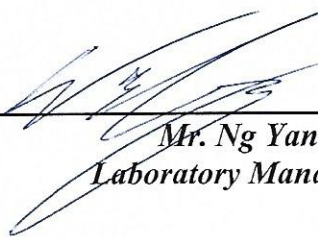**Certified by:**   
**Mr. Ng Yan Wa**  
**Laboratory Manager**

**Date of issue: 27 September 2024**

**Certificate No.: APJ24-072-CC001**



*Page 1 of 4*



**1. Calibration Precaution:**

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

**2. Calibration Conditions:**

Air Temperature: 24.9 °C  
Air Pressure: 1006 hPa  
Relative Humidity: 54.5 %

**3. Calibration Equipment:**

|                          | Type     | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|----------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467    | AV240081                  | HOKLAS       |

**4. Calibration Results**

Sound Pressure Level

Reference Sound Pressure Level

| Setting of Unit-under-test (UUT) |                 |                | Applied value |               | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB                        | Freq. Weighting | Time Weighting | Level, dB     | Frequency, Hz | dB           | Specification, dB |
| 30-130                           | dBA SPL         | Fast           | 94            | 1000          | 94.0         | ±0.4              |

Linearity

| Setting of Unit-under-test (UUT) |                 |                | Applied value |               | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB                        | Freq. Weighting | Time Weighting | Level, dB     | Frequency, Hz | dB           | Specification, dB |
| 30-130                           | dBA SPL         | Fast           | 94            | 1000          | 94.0         | Ref               |
|                                  |                 |                | 104           |               | 104.0        | ±0.3              |
|                                  |                 |                | 114           |               | 114.0        | ±0.3              |

Time Weighting

| Setting of Unit-under-test (UUT) |                 |                | Applied value |               | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB                        | Freq. Weighting | Time Weighting | Level, dB     | Frequency, Hz | dB           | Specification, dB |
| 30-130                           | dBA SPL         | Fast           | 94            | 1000          | 94.0         | Ref               |
|                                  |                 | Slow           |               |               | 94.0         | ±0.3              |

Certificate No.: APJ24-072-CC001



Page 2 of 4

Frequency Response

Linear Response

| Setting of Unit-under-test (UUT) |                 |                | Applied value |               | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB                        | Freq. Weighting | Time Weighting | Level, dB     | Frequency, Hz | dB           | Specification, dB |
| 30-130                           | dB              | SPL            | 94            | 31.5          | 93.8         | $\pm 2.0$         |
|                                  |                 |                |               | 63            | 93.9         | $\pm 1.5$         |
|                                  |                 |                |               | 125           | 93.9         | $\pm 1.5$         |
|                                  |                 |                |               | 250           | 93.9         | $\pm 1.4$         |
|                                  |                 |                |               | 500           | 93.9         | $\pm 1.4$         |
|                                  |                 |                |               | 1000          | 94.0         | Ref               |
|                                  |                 |                |               | 2000          | 94.0         | $\pm 1.6$         |
|                                  |                 |                |               | 4000          | 94.5         | $\pm 1.6$         |
|                                  |                 |                |               | 8000          | 91.8         | +2.1; -3.1        |

A-weighting

| Setting of Unit-under-test (UUT) |                 |                | Applied value |               | UUT Reading, | IEC 61672 Class 1  |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|--------------------|
| Range, dB                        | Freq. Weighting | Time Weighting | Level, dB     | Frequency, Hz | dB           | Specification, dB  |
| 30-130                           | dBA             | SPL            | 94            | 31.5          | 54.4         | $-39.4 \pm 2.0$    |
|                                  |                 |                |               | 63            | 67.8         | $-26.2 \pm 1.5$    |
|                                  |                 |                |               | 125           | 77.8         | $-16.1 \pm 1.5$    |
|                                  |                 |                |               | 250           | 85.3         | $-8.6 \pm 1.4$     |
|                                  |                 |                |               | 500           | 90.7         | $-3.2 \pm 1.4$     |
|                                  |                 |                |               | 1000          | 94.0         | Ref                |
|                                  |                 |                |               | 2000          | 95.2         | $+1.2 \pm 1.6$     |
|                                  |                 |                |               | 4000          | 95.5         | $+1.0 \pm 1.6$     |
|                                  |                 |                |               | 8000          | 90.8         | $-1.1 + 2.1; -3.1$ |

C-weighting

| Setting of Unit-under-test (UUT) |                 |                | Applied value |               | UUT Reading, | IEC 61672 Class 1  |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|--------------------|
| Range, dB                        | Freq. Weighting | Time Weighting | Level, dB     | Frequency, Hz | dB           | Specification, dB  |
| 30-130                           | dBC             | SPL            | 94            | 31.5          | 90.8         | $-3.0 \pm 2.0$     |
|                                  |                 |                |               | 63            | 93.1         | $-0.8 \pm 1.5$     |
|                                  |                 |                |               | 125           | 93.7         | $-0.2 \pm 1.5$     |
|                                  |                 |                |               | 250           | 93.9         | $-0.0 \pm 1.4$     |
|                                  |                 |                |               | 500           | 93.9         | $-0.0 \pm 1.4$     |
|                                  |                 |                |               | 1000          | 94.0         | Ref                |
|                                  |                 |                |               | 2000          | 93.8         | $-0.2 \pm 1.6$     |
|                                  |                 |                |               | 4000          | 93.7         | $-0.8 \pm 1.6$     |
|                                  |                 |                |               | 8000          | 89.0         | $-3.0 + 2.1; -3.1$ |

Certificate No.: APJ24-072-CC001



Page 3 of 4



## 5. *Calibration Results Applied*

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

|        |         |        |
|--------|---------|--------|
| 94 dB  | 31.5 Hz | ± 0.15 |
|        | 63 Hz   | ± 0.10 |
|        | 125 Hz  | ± 0.10 |
|        | 250 Hz  | ± 0.05 |
|        | 500 Hz  | ± 0.10 |
|        | 1000 Hz | ± 0.05 |
|        | 2000 Hz | ± 0.05 |
|        | 4000 Hz | ± 0.05 |
|        | 8000 Hz | ± 0.10 |
| 104 dB | 1000 Hz | ± 0.05 |
| 114 dB | 1000 Hz | ± 0.05 |

The uncertainties are evaluated for a 95% confidence level.

### Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)\*L shall not be liable for any loss or damage resulting from the use of the equipment.

# Certificate of Calibration

## 校正證書

Certificate No. : C242738  
證書編號

ITEM TESTED / 送檢項目 (Job No. / 序引編號 : IC24-0781)

Date of Receipt / 收件日期 : 3 May 2024

Description / 儀器名稱 : Precision Acoustic Calibrator  
Manufacturer / 製造商 : LARSON DAVIS  
Model No. / 型號 : CAL200  
Serial No. / 編號 : 11334  
Supplied By / 委託者 : Envirotech Services Co.  
Room 712, 7/F, My Loft, 9 Hoi Wing Road, Tuen Mun,  
New Territories, Hong Kong

### TEST CONDITIONS / 測試條件

Temperature / 溫度 :  $(23 \pm 2)^{\circ}\text{C}$   
Line Voltage / 電壓 : ---

Relative Humidity / 相對濕度 :  $(50 \pm 25)\%$

### TEST SPECIFICATIONS / 測試規範


Calibration check

DATE OF TEST / 測試日期 : 19 May 2024

### TEST RESULTS / 測試結果

The results apply to the particular unit-under-test only.  
The results do not exceed specified limits.  
These limits refer to manufacturer's published or user's specified tolerances as requested by the customer.  
The results are detailed in the subsequent page(s).

The test equipment used for calibration are traceable to National Standards via :  
- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory  
- Hottinger Brüel & Kjær Calibration Laboratory, Denmark  
- Agilent Technologies / Keysight Technologies  
- Fluke Everett Service Center, USA

Tested By :   
測試 H T Wong  
Assistant Engineer

Certified By :   
核證 K C Lee  
Engineer

Date of Issue : 20 May 2024  
簽發日期

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.  
本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室書面批准。



# Certificate of Calibration

## 校正證書

Certificate No. : C242738  
證書編號

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 12 hours before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.
- Test equipment :

| Equipment ID | Description                       | Certificate No. |
|--------------|-----------------------------------|-----------------|
| CL130        | Universal Counter                 | C233799         |
| CL281        | Multifunction Acoustic Calibrator | CDK2302738      |
| TST150A      | Measuring Amplifier               | C241879         |

- Test procedure : MA100N.

- Results :

### 5.1 Sound Level Accuracy

| UUT<br>Nominal Value | Measured Value<br>(dB) | User's Limit<br>(dB) | Uncertainty of Measured Value<br>(dB) |
|----------------------|------------------------|----------------------|---------------------------------------|
| 94 dB, 1 kHz         | 93.60                  | ± 0.5                | ± 0.20                                |
| 114 dB, 1 kHz        | 113.60                 |                      |                                       |

### 5.2 Frequency Accuracy

| UUT Nominal Value<br>(kHz) | Measured Value<br>(kHz) | Mfr's<br>Limit | Uncertainty of Measured Value<br>(Hz) |
|----------------------------|-------------------------|----------------|---------------------------------------|
| 1                          | 1.000                   | 1 kHz ± 1 %    | ± 1                                   |

Remarks : - The user's limit is a customer pre-defined operating tolerance of the UUT, suitable for one's own intended use.

- The uncertainties are for a confidence probability of not less than 95 %.

Note :

Only the original copy or the laboratory's certified true copy is valid.

The values given in this Certificate only relate to the values measured at the time of the test and any uncertainties quoted will not include allowance for the equipment long term drift, variations with environment changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the measurement. Sun Creation Engineering Limited shall not be liable for any loss or damage resulting from the use of the equipment.

The test equipment used for calibration is traceable to the National Standards as specified in this certificate. This certificate shall not be reproduced except in full, without the prior written approval of this laboratory.

本證書所載校正用之測試器材均可溯源至國際標準。局部複印本證書需先獲本實驗室書面批准。

Sun Creation Engineering Limited - Calibration & Testing Laboratory

c/o 4/F, 1 Hing On Lane, Tuen Mun, New Territories, Hong Kong

輝創工程有限公司 - 校正及檢測實驗室

c/o 香港新界屯門興安里一號四樓

Tel/電話: (852) 2927 2606

Fax/傳真: (852) 2744 8986

E-mail/電郵: callab@suncreation.com

Website/網址: www.suncreation.com