

High-Volume TSP Sampler
5-Point Calibration Record

Location : AM1(ICC)
Calibrated by : K.T.Ho
Date : 04/05/2025

Sampler

Model : TE-5170
Serial Number : S/N 0767

Calibration Orifice and Standard Calibration Relationship

Serial Number : 2454
Next Calibration Date : 02 December 2025
Slope (m) : 2.08315
Intercept (b) : -0.04938
Correlation Coefficient(r) : 0.99985

Standard Condition

Pstd (hpa) : 1013
Tstd (K) : 298.18

Calibration Condition


Pa (hpa) : 1010
Ta(K) : 301

| Resistance Plate | | dH [green liquid] (inch water) | Z | X=Qstd (cubic meter/min) | IC (chart) | Y (corrected) |
|------------------|----------|-----------------------------------|-------|-----------------------------|---------------|------------------|
| 1 | 18 holes | 10.2 | 3.173 | 1.547 | 58 | 57.63 |
| 2 | 13 holes | 7.5 | 2.721 | 1.330 | 50 | 49.68 |
| 3 | 10 holes | 5.6 | 2.351 | 1.152 | 42 | 41.73 |
| 4 | 7 holes | 3.8 | 1.937 | 0.954 | 34 | 33.78 |
| 5 | 5 holes | 2.6 | 1.602 | 0.793 | 24 | 23.85 |

Notes: $Z = \text{SQRT}\{dH(Pa/Pstd)(Tstd/Ta)\}$, $X = Z/m - b$, $Y(\text{Corrected Flow}) = IC * \{\text{SQRT}(Pa/Pstd)(Tstd/Ta)\}$

Sampler Calibration Relationship

Slope(m): 44.098 Intercept(b): -9.6053 Correlation Coefficient(r): 0.9959

Checked by: 
Magnum Fan

Date: 06/05/2025

High-Volume TSP Sampler
5-Point Calibration Record

Location : AM1 (ICC)
Calibrated by : K.T.Ho
Date : 04/07/2025

Sampler

Model : TE-5170
Serial Number : S/N 0767

Calibration Orifice and Standard Calibration Relationship

Serial Number : 2454
Next Calibration Date : 02 December 2025
Slope (m) : 2.08315
Intercept (b) : -0.04938
Correlation Coefficient(r) : 0.99985

Standard Condition

Pstd (hpa) : 1013
Tstd (K) : 298.18

Calibration Condition


Pa (hpa) : 1005
Ta(K) : 305.5

| Resistance Plate | | dH [green liquid] (inch water) | Z | X=Qstd (cubic meter/min) | IC (chart) | Y (corrected) |
|------------------|----------|-----------------------------------|-------|-----------------------------|---------------|------------------|
| 1 | 18 holes | 12.4 | 3.465 | 1.687 | 64 | 62.97 |
| 2 | 13 holes | 9.0 | 2.952 | 1.441 | 54 | 53.13 |
| 3 | 10 holes | 6.6 | 2.528 | 1.237 | 42 | 41.32 |
| 4 | 7 holes | 4.2 | 2.016 | 0.992 | 32 | 31.48 |
| 5 | 5 holes | 2.8 | 1.646 | 0.814 | 20 | 19.68 |

Notes: $Z = \text{SQRT}\{dH(Pa/Pstd)(Tstd/Ta)\}$, $X = Z/m - b$, $Y(\text{Corrected Flow}) = IC * \{\text{SQRT}(Pa/Pstd)(Tstd/Ta)\}$

Sampler Calibration Relationship

Slope(m): 49.113 Intercept(b): -18.891 Correlation Coefficient(r): 0.9967

Checked by: 
Magnum Fan

Date: 07/07/2025

Certificate of Calibration

Calibration Certification Information
Cal. Date: December 2, 2024

Rootsmeter S/N: 438320

Ta: 293

°K
Operator: Jim Tisch

Pa: 757.4

mm Hg
Calibration Model #: TE-5025A

Calibrator S/N: 2454

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|-------------------|--------------------|---------------|----------------|---------------|----------------|
| 1 | 1 | 2 | 1 | 1.4200 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0170 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9090 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8700 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7140 | 12.8 | 8.00 |

Data Tabulation

| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis) |
|--------------|------------------|---|-----------|----------------|--|
| 1.0093 | 0.7108 | 1.4238 | 0.9958 | 0.7013 | 0.8796 |
| 1.0051 | 0.9883 | 2.0136 | 0.9916 | 0.9750 | 1.2439 |
| 1.0031 | 1.1035 | 2.2512 | 0.9896 | 1.0886 | 1.3907 |
| 1.0018 | 1.1515 | 2.3611 | 0.9884 | 1.1361 | 1.4586 |
| 0.9965 | 1.3956 | 2.8476 | 0.9831 | 1.3769 | 1.7592 |
| QSTD | m= | 2.08315 | QA | m= | 1.30443 |
| | b= | -0.04938 | | b= | -0.03050 |
| | r= | 0.99985 | | r= | 0.99985 |

Calculations

| | | | |
|--|---|---|--------------------------------|
| Vstd= | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$ | Va= | $\Delta Vol((Pa-\Delta P)/Pa)$ |
| Qstd= | $Vstd/\Delta Time$ | Qa= | $Va/\Delta Time$ |
| For subsequent flow rate calculations: | | | |
| Qstd= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | | Qa= $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$ | |

Standard Conditions

| | |
|---|-----------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: calibrator manometer reading (in H2O) | |
| ΔP: rootsmeter manometer reading (mm Hg) | |
| Ta: actual absolute temperature (°K) | |
| Pa: actual barometric pressure (mm Hg) | |
| b: intercept | |
| m: slope | |

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



SUB-CONTRACTING REPORT

| | | | |
|---------|--|----------------|--------------------|
| CONTACT | : MR MAGNUM FAN | WORK ORDER | : HK2502565 |
| CLIENT | : ENVIROTECH SERVICES CO. | | |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD, TUEN MUN, N.T. HK | SUB-BATCH | : 1 |
| | | DATE RECEIVED | : 15-JAN-2025 |
| | | DATE OF ISSUE | : 21-JAN-2025 |
| PROJECT | : ---- | NO. OF SAMPLES | : 1 |
| | | CLIENT ORDER | : ---- |

General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
 - Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
 - Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
 - Calibration was subcontracted to Envirotech Services Company.
-

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong
Tel. +852 2610 1044 Fax. +852 2610 2021 www.alsglobal.com

WORK ORDER : HK2502565
SUB-BATCH : 1
CLIENT : ENVIROTECH SERVICES CO.
PROJECT : ----



| ALS Lab ID | Client's Sample ID | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2502565-001 | Sibata LD-5R (831656) | Equipments | 02-Jan-2025 | S/N: 831656 |

----- END OF REPORT -----



Envirotech Services Co.

Rm. 712, 7/F
My Loft,
9 Hoi Wing Road,
Tuen Mun, H.K.
Tel : 2560 8450
Fax : 2560 6553
E-mail: envirotech@netvigator.com

Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust Monitor
Manufacturer: Sibata LD-5R
Serial No.: 831656
Equipment Ref.: N/A
ALS Job Order: HK2500343

Standard Equipment

Standard Equipment: High Volume Sampler (TSP)
Location: Envirotech Room (Calibration Room)
Equipment Ref.: HVS 8162
Last Calibration Date: 1-Jan-2025


Equipment Verification Results:

Verification Date: 2-Jan-2025

| Hour | Time | Mean Temp °C | Mean Pressure (hpa) | TSP Level in mg (Standard Equipment) (Y-Axis) | Total Count (Calibrated Equipment) (X-Axis) |
|------------|-----------|-----------------|---------------------------|---|---|
| 1hr 00mins | 0900-1000 | 16.1 | 1023 | 0.096 | 62 |
| 2hr 00mins | 1005-1205 | 20.5 | 1022 | 0.147 | 122 |
| 3hr 00mins | 1330-1630 | 21.0 | 1022 | 0.268 | 220 |

Linear Regression of Y or X

Slope (K-factor): 0.0012(mg)/Count
Correlation Coefficient (R): 0.9959
Date of Issue: 15-Jan-2025

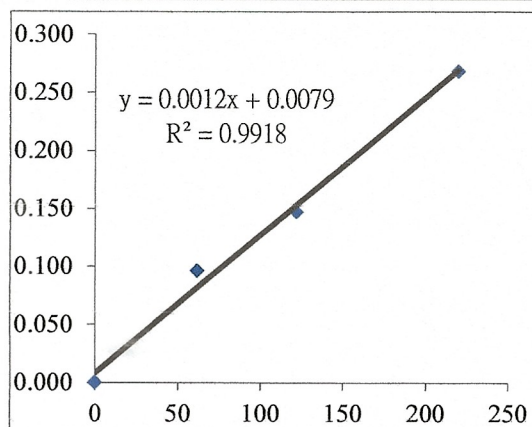

Remarks:

1. Strong Correlation (>0.8)
2. Factor 0.0012(mg)/Count should be applied for TSP monitoring

*If $R < 0.5$, repair or verification is required for the equipment

Operator: P.F.Yeung Signature Fai Date: 15 Jan 2025

QC Reviewer: K.F.Ho Signature at Date: 15 Jan 2025

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location : Rm. 712, My Loft, Tuen Mun Date of Calibration: 1-Jan-25
HVS ID: 8162 Next Calibration Date: 31-Mar-25
Name and Model : TISCH HVS Model TE-5170 Operator: K.F.Ho

CONDITIONS

| | | | |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1023 | Corrected Pressure (mm Hg) | 767.3 |
| Temperature (°C) | 15.8 | Temperature (K) | 288.8 |

CALIBRATION ORIFICE

| | | | |
|----------|----------|----------------|----------|
| Make: | TISCH | Qstd Slope | 2.08315 |
| Model: | TE-5025A | Qstd Intercept | -0.04938 |
| Serial#: | 2454 | | |

CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|---|
| 18 | 6.4 | 6.4 | 12.8 | 1.777 | 62 | 63.30 | Slope= 35.208 Intercept= -0.0015 Corr. Coeff.= 0.9959 |
| 13 | 5.3 | 5.3 | 10.6 | 1.619 | 56 | 57.17 | |
| 10 | 4.2 | 4.2 | 8.4 | 1.444 | 48 | 49.00 | |
| 7 | 2.7 | 2.7 | 5.4 | 1.163 | 41 | 41.86 | |
| 5 | 1.7 | 1.7 | 3.4 | 0.927 | 32 | 32.67 | |

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I) [\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

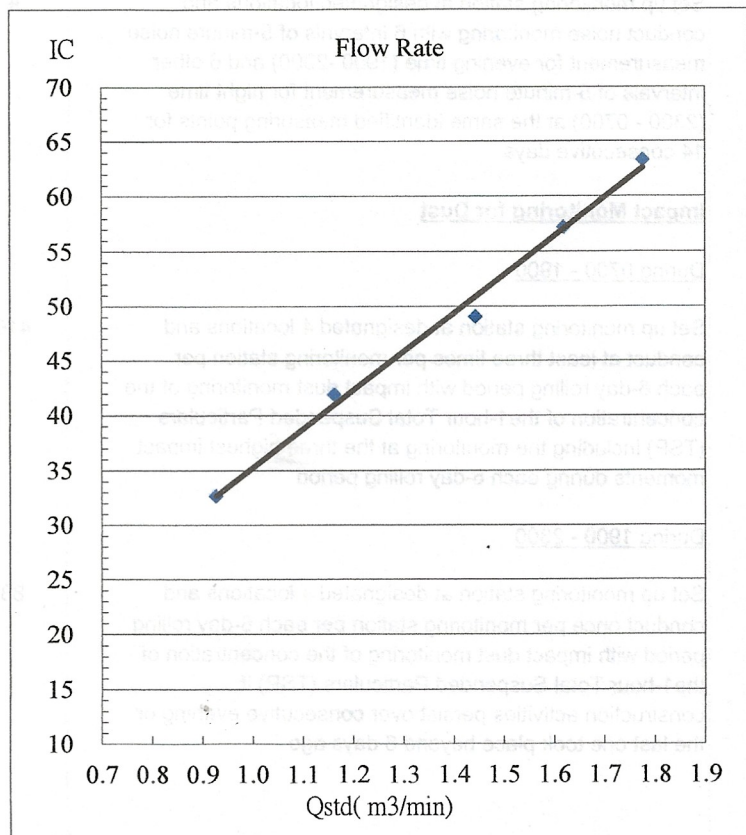

Certificate of Calibration

Calibration Certification Information

Cal. Date: December 2, 2024

Rootsmeter S/N: 438320

Ta: 293 °K

Operator: Jim Tisch

Pa: 757.4 mm Hg

Calibration Model #: TE-5025A

Calibrator S/N: 2454

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4200 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0170 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9090 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8700 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7140 | 12.8 | 8.00 |

Data Tabulation

| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis) |
|-------------|---------------|--|-----------|-------------|---|
| 1.0093 | 0.7108 | 1.4238 | 0.9958 | 0.7013 | 0.8796 |
| 1.0051 | 0.9883 | 2.0136 | 0.9916 | 0.9750 | 1.2439 |
| 1.0031 | 1.1035 | 2.2512 | 0.9896 | 1.0886 | 1.3907 |
| 1.0018 | 1.1515 | 2.3611 | 0.9884 | 1.1361 | 1.4586 |
| 0.9965 | 1.3956 | 2.8476 | 0.9831 | 1.3769 | 1.7592 |
| QSTD | m= | 2.08315 | QA | m= | 1.30443 |
| | b= | -0.04938 | | b= | -0.03050 |
| | r= | 0.99985 | | r= | 0.99985 |

Calculations

| | | | |
|--|---|-----|--|
| Vstd= | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$ | Va= | $\Delta Vol((Pa-\Delta P)/Pa)$ |
| Qstd= | Vstd/ΔTime | Qa= | Va/ΔTime |
| For subsequent flow rate calculations: | | | |
| Qstd= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$ |

Standard Conditions

| | |
|---|-----------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: calibrator manometer reading (in H2O) | |
| ΔP: rootsmeter manometer reading (mm Hg) | |
| Ta: actual absolute temperature (°K) | |
| Pa: actual barometric pressure (mm Hg) | |
| b: intercept | |
| m: slope | |

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



SUB-CONTRACTING REPORT

CONTACT : MR MAGNUM FAN
CLIENT : ENVIROTECH SERVICES CO.
ADDRESS : RM 712, 7/F, MY LOFT 9 HOI WING ROAD,
TUEN MUN, N.T. HK
PROJECT : ---

WORK ORDER : HK2500019
SUB-BATCH : 1
DATE RECEIVED : 16-DEC-2024
DATE OF ISSUE : 8-JAN-2025
NO. OF SAMPLES : 1
CLIENT ORDER : ---

General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
- Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
- Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
- Calibration was subcontracted to Envirotech Services Company.

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong
Tel. +852 2610 1044 Fax. +852 2610 2021 www.alsglobal.com

WORK ORDER : HK2500019
SUB-BATCH : 1
CLIENT : ENVIROTECH SERVICES CO.
PROJECT : ----



| ALS Lab ID | Client's Sample ID | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2500019-001 | Sibata LD-3B (235780) | Equipments | 07-Dec-2024 | S/N: 235780 |

----- END OF REPORT -----



Envirotech Services Co.

Rm. 712, 7/F
My Loft,
9 Hoi Wing Road,
Tuen Mun, H.K.
Tel : 2560 8450
Fax : 2560 6553
E mail: envirotech@netvigator.com

Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust Monitor
Manufacturer: Sibata LD-3B
Serial No.: 235780
Equipment Ref.: N/A
ALS Job Order: HK2451037

Standard Equipment

Standard Equipment: High Volume Sampler (TSP)
Location: Envirotech Room (Calibration Room)
Equipment Ref.: HVS 8162
Last Calibration Date: 19-Oct-2024


Equipment Verification Results:

Verification Date: 7-Dec-2024

| Hour | Time | Mean Temp °C | Mean Pressure (hpa) | Concentration in $\mu\text{g}/\text{m}^3$ (Standard Equipment) (Y-Axis) | Concentration in $\mu\text{g}/\text{m}^3$ (Calibrated Equipment) (X-Axis) |
|------------|-----------|--------------|---------------------|---|---|
| 1hr 00mins | 0910-1010 | 19.5 | 1022 | 84 | 72 |
| 2hr 00mins | 1300-1500 | 21.2 | 1019 | 177 | 150 |
| 3hr 00mins | 1505-1805 | 21.5 | 1018 | 223 | 195 |

Linear Regression of Y or X

Slope (K-factor): $1.1524(\mu\text{g}/\text{m}^3)/\text{CPM}$
Correlation Coefficient (R): 0.9997
Date of Issue: 14-Dec-2024

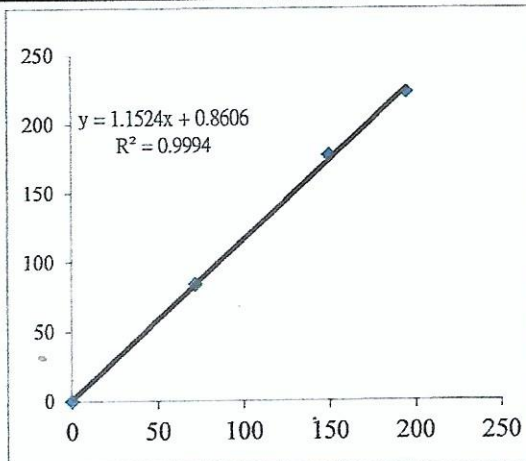

Remarks:

1. Strong Correlation (>0.8)
2. Factor $1.1524(\mu\text{g}/\text{m}^3)/\text{CPM}$ should be applied for TSP monitoring

*If $R < 0.5$, repair or verification is required for the equipment

Operator: P.F.Yeung Signature *Pa?* Date: 14 Dec 2024

QC Reviewer: K.F.Ho Signature *at* Date: 14 Dec 2024

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

| | | |
|--|------------------------|-----------|
| Location : Rm. 712, My Loft, Tuen Mun | Date of Calibration: | 19-Oct-24 |
| HVS ID: 8162 | Next Calibration Date: | 19-Dec-24 |
| Name and Model : TISCH HVS Model TE-5170 | Operator: | K.F.Ho |

CONDITIONS

| | | | |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1015 | Corrected Pressure (mm Hg) | 761.3 |
| Temperature (°C) | 26.0 | Temperature (K) | 299 |

CALIBRATION ORIFICE

| | | | |
|----------|----------|----------------|----------|
| Make: | TISCH | Qstd Slope | 2.07544 |
| Model: | TE-5025A | Qstd Intercept | -0.03205 |
| Serial#: | 2454 | | |

CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|--|
| 18 | 6.1 | 6.4 | 12.5 | 1.718 | 62 | 61.97 | Slope= 45.67 Intercept= -15.103 Corr. Coeff.= 0.9947 |
| 13 | 4.9 | 5.2 | 10.1 | 1.546 | 56 | 55.97 | |
| 10 | 3.6 | 3.8 | 7.4 | 1.325 | 48 | 47.97 | |
| 7 | 2.4 | 2.7 | 5.1 | 1.103 | 34 | 33.98 | |
| 5 | 1.4 | 1.7 | 3.1 | 0.863 | 24 | 23.99 | |

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m(I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

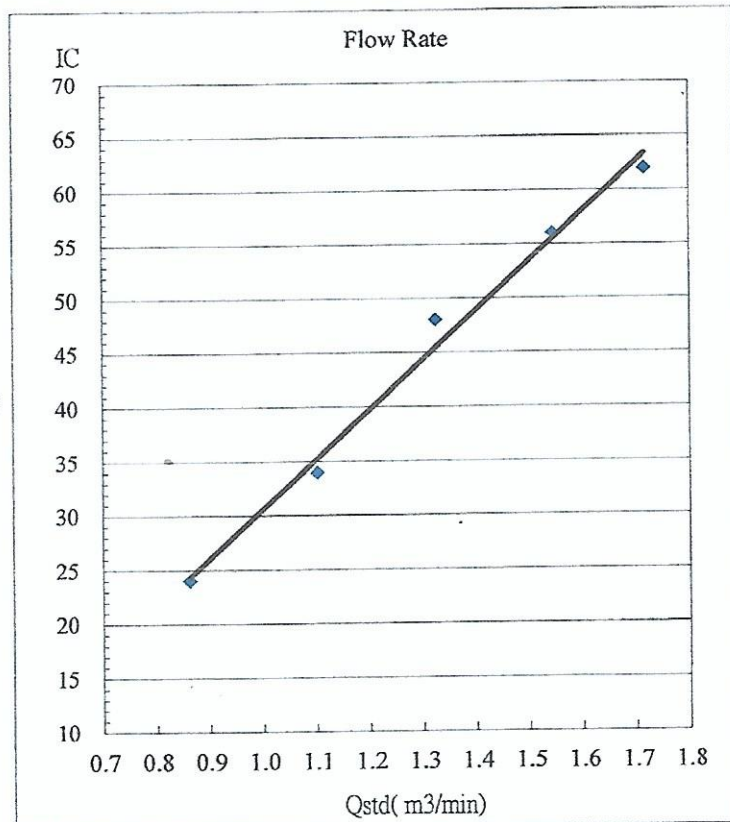

Certificate of Calibration

Calibration Certification Information

Cal. Date: December 15, 2023 **Rootsmeter S/N:** 438320 **Ta:** 295 °K
Operator: Jim Tisch **Pa:** 748.5 mm Hg
Calibration Model #: TE-5025A **Calibrator S/N:** 2454

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4250 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0090 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9040 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8610 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7110 | 12.8 | 8.00 |

Data Tabulation

| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis) |
|-------------|---------------|--|-----------|-------------|---|
| 0.9907 | 0.6952 | 1.4106 | 0.9957 | 0.6988 | 0.8878 |
| 0.9864 | 0.9776 | 1.9949 | 0.9914 | 0.9826 | 1.2556 |
| 0.9844 | 1.0890 | 2.2304 | 0.9894 | 1.0945 | 1.4037 |
| 0.9832 | 1.1420 | 2.3393 | 0.9882 | 1.1478 | 1.4723 |
| 0.9779 | 1.3754 | 2.8213 | 0.9829 | 1.3824 | 1.7756 |
| QSTD | m= | 2.07544 | QA | m= | 1.29961 |
| | b= | -0.03205 | | b= | -0.02017 |
| | r= | 0.99999 | | r= | 0.99999 |

Calculations

| | | | |
|---|---|------------|--|
| Vstd= | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$ | Va= | $\Delta Vol((Pa-\Delta P)/Pa)$ |
| Qstd= | $Vstd/\Delta Time$ | Qa= | $Va/\Delta Time$ |
| For subsequent flow rate calculations: | | | |
| Qstd= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$ |

Standard Conditions

| | |
|---|-----------|
| Tstd: | 298.15 °K |
| Pstd: | 760 mm Hg |
| Key | |
| ΔH: calibrator manometer reading (in H2O) | |
| ΔP: rootsmeter manometer reading (mm Hg) | |
| Ta: actual absolute temperature (°K) | |
| Pa: actual barometric pressure (mm Hg) | |
| b: intercept | |
| m: slope | |

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30



SUB-CONTRACTING REPORT

| | | | |
|---------|--|----------------|---------------|
| CONTACT | : MR MAGNUM FAN | WORK ORDER | : HK2448121 |
| CLIENT | : ENVIROTECH SERVICES CO. | | |
| ADDRESS | : RM 712, 7/F, MY LOFT 9 HOI WING ROAD, TUEN MUN, N.T. HK | SUB-BATCH | : 1 |
| | | DATE RECEIVED | : 13-NOV-2024 |
| | | DATE OF ISSUE | : 20-NOV-2024 |
| PROJECT | : ---- | NO. OF SAMPLES | : 1 |
| | | CLIENT ORDER | : ---- |

General Comments

- Sample information (Project name, Sample ID, Sampling date/time, etc.) is provided by client.
- Result(s) of sample(s) is/are reported on as received basis, unless otherwise specified. The result(s) is/are related only to the item(s) tested.
- Sample(s) was/ were submitted by client. Sample(s) arrived laboratory in ambient condition.
- Calibration was subcontracted to Envirotech Services Company.

Signatories

This document has been signed by those names that appear on this report and are the authorised signatories

Signatories

Position

Richard Fung

Managing Director

This report supersedes any previous report(s) with the same work order number.

All pages of this report have been checked and approved for release.

ALS Technichem (HK) Pty Ltd
Part of the **ALS Laboratory Group**

11/F, Chung Shun Knitting Centre 1 - 3 Wing Yip Street Kwai Chung N.T. Hong Kong
Tel. +852 2610 1044 Fax. +852 2610 2021 www.alsglobal.com

WORK ORDER : HK2448121
SUB-BATCH : 1
CLIENT : ENVIROTECH SERVICES CO.
PROJECT : ----



| ALS Lab ID | Client's Sample ID | Sample Type | Sample Date | External Lab Report No. |
|---------------|-----------------------|-------------|-------------|-------------------------|
| HK2448121-001 | Sibata LD-3B (245834) | Equipments | 09-Nov-2024 | S/N: 245834 |

----- END OF REPORT -----



Equipment Verification Report (TSP)

Equipment Calibrated:

Type: Laser Dust Monitor
Manufacturer: Sibata LD-3B
Serial No.: 245834
Equipment Ref.: N/A
ALS Job Order: HK2446853

Standard Equipment

Standard Equipment: High Volume Sampler (TSP)
Location: Envirotech Room (Calibration Room)
Equipment Ref.: HVS 8162
Last Calibration Date: 19-Oct-2024


Equipment Verification Results:

Verification Date: 9-Nov-2024

| Hour | Time | Mean Temp °C | Mean Pressure (hpa) | Concentration in $\mu\text{g}/\text{m}^3$ (Standard Equipment) (Y-Axis) | Concentration in $\mu\text{g}/\text{m}^3$ (Calibrated Equipment) (X-Axis) |
|------------|-----------|-----------------|---------------------------|---|---|
| 1hr 00mins | 0905-1005 | 24.9 | 1013 | 85 | 104 |
| 2hr 00mins | 1015-1215 | 25.2 | 1014 | 155 | 193 |
| 3hr 00mins | 1430-1730 | 25.6 | 1014 | 196 | 250 |

Linear Regression of Y or X

Slope (K-factor): $1.2705(\mu\text{g}/\text{m}^3)/\text{CPM}$
Correlation Coefficient (R): 0.9997
Date of Issue: 13-Nov-2024

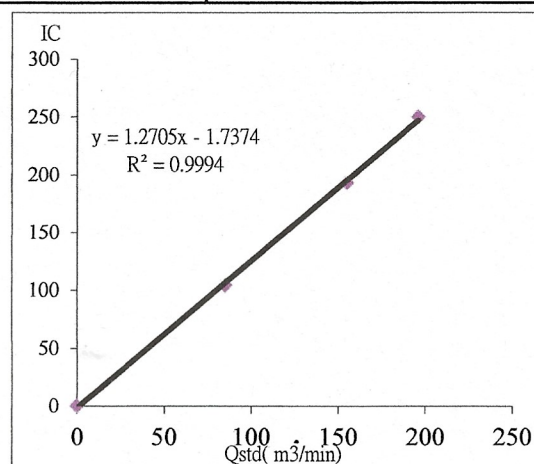

Remarks:

1. Strong Correlation (>0.8)
2. Factor $1.2705(\mu\text{g}/\text{m}^3)/\text{CPM}$ should be applied for TSP monitoring

*If $R < 0.5$, repair or verification is required for the equipment

Operator: P.F.Yeung Signature Date: 11 Nov 2024

QC Reviewer: K.F.Ho Signature Date: 11 Nov 2024

TSP SAMPLER CALIBRATION CALCULATION SPREADSHEET

Location : Rm. 712, My Loft, Tuen Mun Date of Calibration: 19-Oct-24
HVS ID: 8162 Next Calibration Date: 19-Dec-24
Name and Model : TISCH HVS Model TE-5170 Operator: K.F.Ho

CONDITIONS

| | | | |
|--------------------------|------|----------------------------|-------|
| Sea Level Pressure (hpa) | 1015 | Corrected Pressure (mm Hg) | 761.3 |
| Temperature (°C) | 26.0 | Temperature (K) | 299 |

CALIBRATION ORIFICE

| | | | |
|----------|----------|----------------|----------|
| Make: | TISCH | Qstd Slope | 2.07544 |
| Model: | TE-5025A | Qstd Intercept | -0.03205 |
| Serial#: | 2454 | | |

CALIBRATION

| Plate No. | H2O(L) (in) | H2O(R) (in) | H2O (in) | Qstd (m3/min) | I (chart) | IC (corrected) | LINEAR REGRESSION |
|-----------|-------------|-------------|----------|---------------|-----------|----------------|--|
| 18 | 6.1 | 6.4 | 12.5 | 1.718 | 62 | 61.97 | Slope= 45.67 Intercept= -15.103 Corr. Coeff.= 0.9947 |
| 13 | 4.9 | 5.2 | 10.1 | 1.546 | 56 | 55.97 | |
| 10 | 3.6 | 3.8 | 7.4 | 1.325 | 48 | 47.97 | |
| 7 | 2.4 | 2.7 | 5.1 | 1.103 | 34 | 33.98 | |
| 5 | 1.4 | 1.7 | 3.1 | 0.863 | 24 | 23.99 | |

Calculations:

$$Qstd = 1/m[\text{Sqrt}(H2O(Pa/Pstd)(Tstd/Ta))-b]$$

$$IC = I[\text{Sqrt}(Pa/Pstd)(Tstd/Ta)]$$

Qstd = standard flow rate

IC = corrected chart response

I = actual chart response

m = calibrator Qstd slope

b = calibrator Qstd intercept

Ta = actual temperature during calibration (deg K)

Pa = actual pressure during calibration (mm Hg)

For subsequent calculation of sampler flow:

$$1/m((I[\text{Sqrt}(298/Tav)(Pav/760)]-b)$$


m = sampler slope

b = sampler intercept

I = chart response

Tav = daily average temperature

Pav = daily average pressure

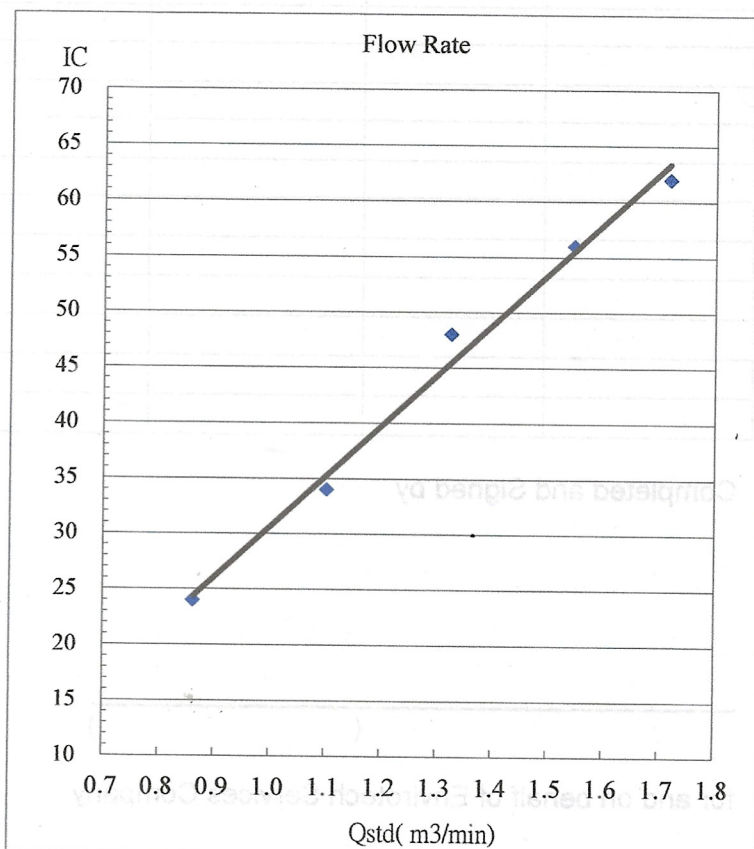

Certificate of Calibration

Calibration Certification Information

Cal. Date: December 15, 2023 Rootsmeter S/N: 438320 Ta: 295 °K
 Operator: Jim Tisch Pa: 748.5 mm Hg
 Calibration Model #: TE-5025A Calibrator S/N: 2454

| Run | Vol. Init (m3) | Vol. Final (m3) | ΔVol. (m3) | ΔTime (min) | ΔP (mm Hg) | ΔH (in H2O) |
|-----|----------------|-----------------|------------|-------------|------------|-------------|
| 1 | 1 | 2 | 1 | 1.4250 | 3.2 | 2.00 |
| 2 | 3 | 4 | 1 | 1.0090 | 6.4 | 4.00 |
| 3 | 5 | 6 | 1 | 0.9040 | 7.9 | 5.00 |
| 4 | 7 | 8 | 1 | 0.8610 | 8.8 | 5.50 |
| 5 | 9 | 10 | 1 | 0.7110 | 12.8 | 8.00 |

Data Tabulation

| Vstd (m3) | Qstd (x-axis) | $\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)}$ (y-axis) | Va | Qa (x-axis) | $\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)}$ (y-axis) |
|-------------|---------------|--|-----------|-------------|---|
| 0.9907 | 0.6952 | 1.4106 | 0.9957 | 0.6988 | 0.8878 |
| 0.9864 | 0.9776 | 1.9949 | 0.9914 | 0.9826 | 1.2556 |
| 0.9844 | 1.0890 | 2.2304 | 0.9894 | 1.0945 | 1.4037 |
| 0.9832 | 1.1420 | 2.3393 | 0.9882 | 1.1478 | 1.4723 |
| 0.9779 | 1.3754 | 2.8213 | 0.9829 | 1.3824 | 1.7756 |
| QSTD | m= | 2.07544 | QA | m= | 1.29961 |
| | b= | -0.03205 | | b= | -0.02017 |
| | r= | 0.99999 | | r= | 0.99999 |

Calculations

| | | | |
|--|---|-----|--|
| Vstd= | $\Delta Vol((Pa-\Delta P)/Pstd)(Tstd/Ta)$ | Va= | $\Delta Vol((Pa-\Delta P)/Pa)$ |
| Qstd= | Vstd/ΔTime | Qa= | Va/ΔTime |
| For subsequent flow rate calculations: | | | |
| Qstd= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Pa}{Pstd} \right) \left(\frac{Tstd}{Ta} \right)} \right) - b \right)$ | Qa= | $1/m \left(\left(\sqrt{\Delta H \left(\frac{Ta}{Pa} \right)} \right) - b \right)$ |

Standard Conditions

Tstd: 298.15 °K

Pstd: 760 mm Hg

Key

ΔH: calibrator manometer reading (in H2O)
 ΔP: rootsmeter manometer reading (mm Hg)
 Ta: actual absolute temperature (°K)
 Pa: actual barometric pressure (mm Hg)
 b: intercept
 m: slope

RECALIBRATION

US EPA recommends annual recalibration per 1998 40 Code of Federal Regulations Part 50 to 51, Appendix B to Part 50, Reference Method for the Determination of Suspended Particulate Matter in the Atmosphere, 9.2.17, page 30

Certificate of Calibration

for

Description: Sound Level Calibrator

Manufacturer: Larson Davis

Type No.: CAL200

Serial No.: 16172

Submitted by:

Customer: Envirotech Services Co.

Address: Rm.712, 7/F., My Loft, 9 Hoi Wing Road,
Tuen Mun, Hong Kong

Upon receipt for calibration, the instrument was found to be:

☒ Within

☐ Outside

the allowable tolerance.

The test equipments used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 6 February 2025

Date of calibration: 7 February 2025

Date of NEXT calibration: 6 February 2026

Calibrated by: 
Calibration Technician

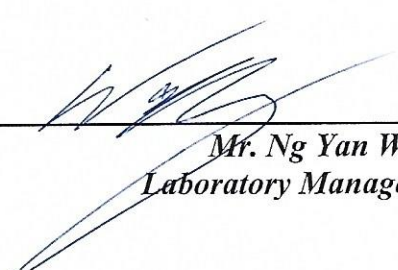Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 7 February 2025

Certificate No.: APJ24-143-CC002



Page 1 of 2

1. Calibration Precautions:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Specifications:

Calibration check

3. Calibration Conditions:

Air Temperature: 24.3 °C
Air Pressure: 1006 hPa
Relative Humidity: 59.2 %

4. Calibration Equipment:

| Test Equipment | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|------------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV240081 | HOKLAS |
| Sound Level Meter | RION NA-28 | 30721812 | AV240109 | HOKLAS |

5. Calibration Results**5.1 Sound Pressure Level**

| Nominal value dB | Accept lower level dB | Accept upper level dB | Measured value dB |
|---------------------|--------------------------|--------------------------|----------------------|
| 94.0 | 93.6 | 94.4 | 93.7 |
| 114.0 | 113.6 | 114.4 | 113.7 |

6. Calibration Results Applied

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 60942 Class 1.

Note:

The values given in this certification only related to the values measured at the time of the calibration.

Certificate No.: APJ24-143-CC002



Page 2 of 2

Certificate of Calibration

for

Description: **Sound Level Meter**
Manufacturer: **RION**
Type No.: **NL-52 (Serial No.: 00643040)**
Microphone: **PCB 377B02 (Serial No.: 172764)**
Preamplifier: **NH-25 (Serial No.: 21757)**

Submitted by:

Customer: **Envirotech Services Co.**
Address: **Rm. 712, 7/F., My Loft, 9 Hoi Wing Road,
Tuen Mun, Hong Kong**

Upon receipt for calibration, the instrument was found to be:

- ☒ **Within (31.5Hz – 8kHz)**
☐ **Outside**

the allowable tolerance.

The test equipment used for calibration are traceable to National Standards via:


- The Government of The Hong Kong Special Administrative Region Standard & Calibration Laboratory

Date of receipt: 25 September 2024

Date of calibration: 27 September 2024

Date of NEXT calibration: 26 September 2025

Calibrated by: 
Calibration Technician

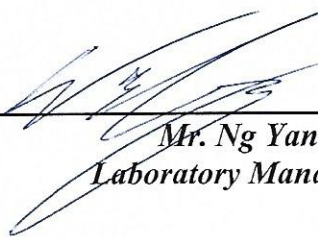Certified by: 
Mr. Ng Yan Wa
Laboratory Manager

Date of issue: 27 September 2024

Certificate No.: APJ24-072-CC001



Page 1 of 4

1. Calibration Precaution:

- The unit-under-test (UUT) was allowed to stabilize in the laboratory for over 24 hours, and switched on to warm up for over 10 minutes before the commencement of the test.
- The results presented are the mean of 3 measurements at each calibration point.

2. Calibration Conditions:

Air Temperature: 24.9 °C
Air Pressure: 1006 hPa
Relative Humidity: 54.5 %

3. Calibration Equipment:

| | Type | Serial No. | Calibration Report Number | Traceable to |
|--------------------------|----------|------------|---------------------------|--------------|
| Multifunction Calibrator | B&K 4226 | 2288467 | AV240081 | HOKLAS |

4. Calibration Results

Sound Pressure Level

Reference Sound Pressure Level

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.0 | ±0.4 |

Linearity

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.0 | Ref |
| | | | 104 | | 104.0 | ±0.3 |
| | | | 114 | | 114.0 | ±0.3 |

Time Weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 30-130 | dBA SPL | Fast | 94 | 1000 | 94.0 | Ref |
| | | Slow | | | 94.0 | ±0.3 |

Certificate No.: APJ24-072-CC001



Page 2 of 4

Frequency Response

Linear Response

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|-------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 30-130 | dB | SPL | 94 | 31.5 | 93.8 | ± 2.0 |
| | | | | 63 | 93.9 | ± 1.5 |
| | | | | 125 | 93.9 | ± 1.5 |
| | | | | 250 | 93.9 | ± 1.4 |
| | | | | 500 | 93.9 | ± 1.4 |
| | | | | 1000 | 94.0 | Ref |
| | | | | 2000 | 94.0 | ± 1.6 |
| | | | | 4000 | 94.5 | ± 1.6 |
| | | | | 8000 | 91.8 | +2.1; -3.1 |

A-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|--------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 30-130 | dBA | SPL | 94 | 31.5 | 54.4 | -39.4 ± 2.0 |
| | | | | 63 | 67.8 | -26.2 ± 1.5 |
| | | | | 125 | 77.8 | -16.1 ± 1.5 |
| | | | | 250 | 85.3 | -8.6 ± 1.4 |
| | | | | 500 | 90.7 | -3.2 ± 1.4 |
| | | | | 1000 | 94.0 | Ref |
| | | | | 2000 | 95.2 | $+1.2 \pm 1.6$ |
| | | | | 4000 | 95.5 | $+1.0 \pm 1.6$ |
| | | | | 8000 | 90.8 | $-1.1 + 2.1; -3.1$ |

C-weighting

| Setting of Unit-under-test (UUT) | | | Applied value | | UUT Reading, | IEC 61672 Class 1 |
|----------------------------------|-----------------|----------------|---------------|---------------|--------------|--------------------|
| Range, dB | Freq. Weighting | Time Weighting | Level, dB | Frequency, Hz | dB | Specification, dB |
| 30-130 | dBC | SPL | 94 | 31.5 | 90.8 | -3.0 ± 2.0 |
| | | | | 63 | 93.1 | -0.8 ± 1.5 |
| | | | | 125 | 93.7 | -0.2 ± 1.5 |
| | | | | 250 | 93.9 | -0.0 ± 1.4 |
| | | | | 500 | 93.9 | -0.0 ± 1.4 |
| | | | | 1000 | 94.0 | Ref |
| | | | | 2000 | 93.8 | -0.2 ± 1.6 |
| | | | | 4000 | 93.7 | -0.8 ± 1.6 |
| | | | | 8000 | 89.0 | $-3.0 + 2.1; -3.1$ |

Certificate No.: APJ24-072-CC001



Page 3 of 4

5. *Calibration Results Applied*

The results apply to the particular unit-under-test only. All calibration points are within manufacture's specification as IEC 61672 Class 1.

Uncertainties of Applied Value:

| | | |
|--------|---------|--------|
| 94 dB | 31.5 Hz | ± 0.15 |
| | 63 Hz | ± 0.10 |
| | 125 Hz | ± 0.10 |
| | 250 Hz | ± 0.05 |
| | 500 Hz | ± 0.10 |
| | 1000 Hz | ± 0.05 |
| | 2000 Hz | ± 0.05 |
| | 4000 Hz | ± 0.05 |
| | 8000 Hz | ± 0.10 |
| 104 dB | 1000 Hz | ± 0.05 |
| 114 dB | 1000 Hz | ± 0.05 |

The uncertainties are evaluated for a 95% confidence level.

Note:

The values given in this certification only related to the values measured at the time of the calibration and any uncertainties quoted will not allow for the equipment long-term drift, variations with environmental changes, vibration and shock during transportation, overloading, mis-handling, or the capability of any other laboratory to repeat the calibration. (A+A)*L shall not be liable for any loss or damage resulting from the use of the equipment.